



Canada's Drug and
Health Technology Agency

CDA-AMC Health Technology Review

RapidAI for Stroke Detection: Supporting Information

August 2024



Table of Contents

Abbreviations	3
Selection of Included Studies	4
List of Included Publications	5
List of Excluded Publications and Reasons for Exclusion	6
Characteristics of Included Publications	11
Critical Appraisal of Included Studies	17
Main Study Findings.....	46
Reasons for Certainty of Evidence Ratings	57
Patient Engagement.....	60
References.....	62

DRAFT



Abbreviations


AI	artificial intelligence
ICH	intracranial hemorrhage
LVO	large vessel occlusion
QUADAS-2	Quality Assessment of Diagnostic Accuracy Studies 2
ROBINS-I	Risk Of Bias In Nonrandomized Studies – of Interventions

DRAFT

Selection of Included Studies

Figure 1: Selection of Included Studies

Alt text: 309 citations were identified, 242 were excluded, while 67 electronic literature and 20 additional potentially relevant full text reports were retrieved for scrutiny. In total 11 reports are included in the review.

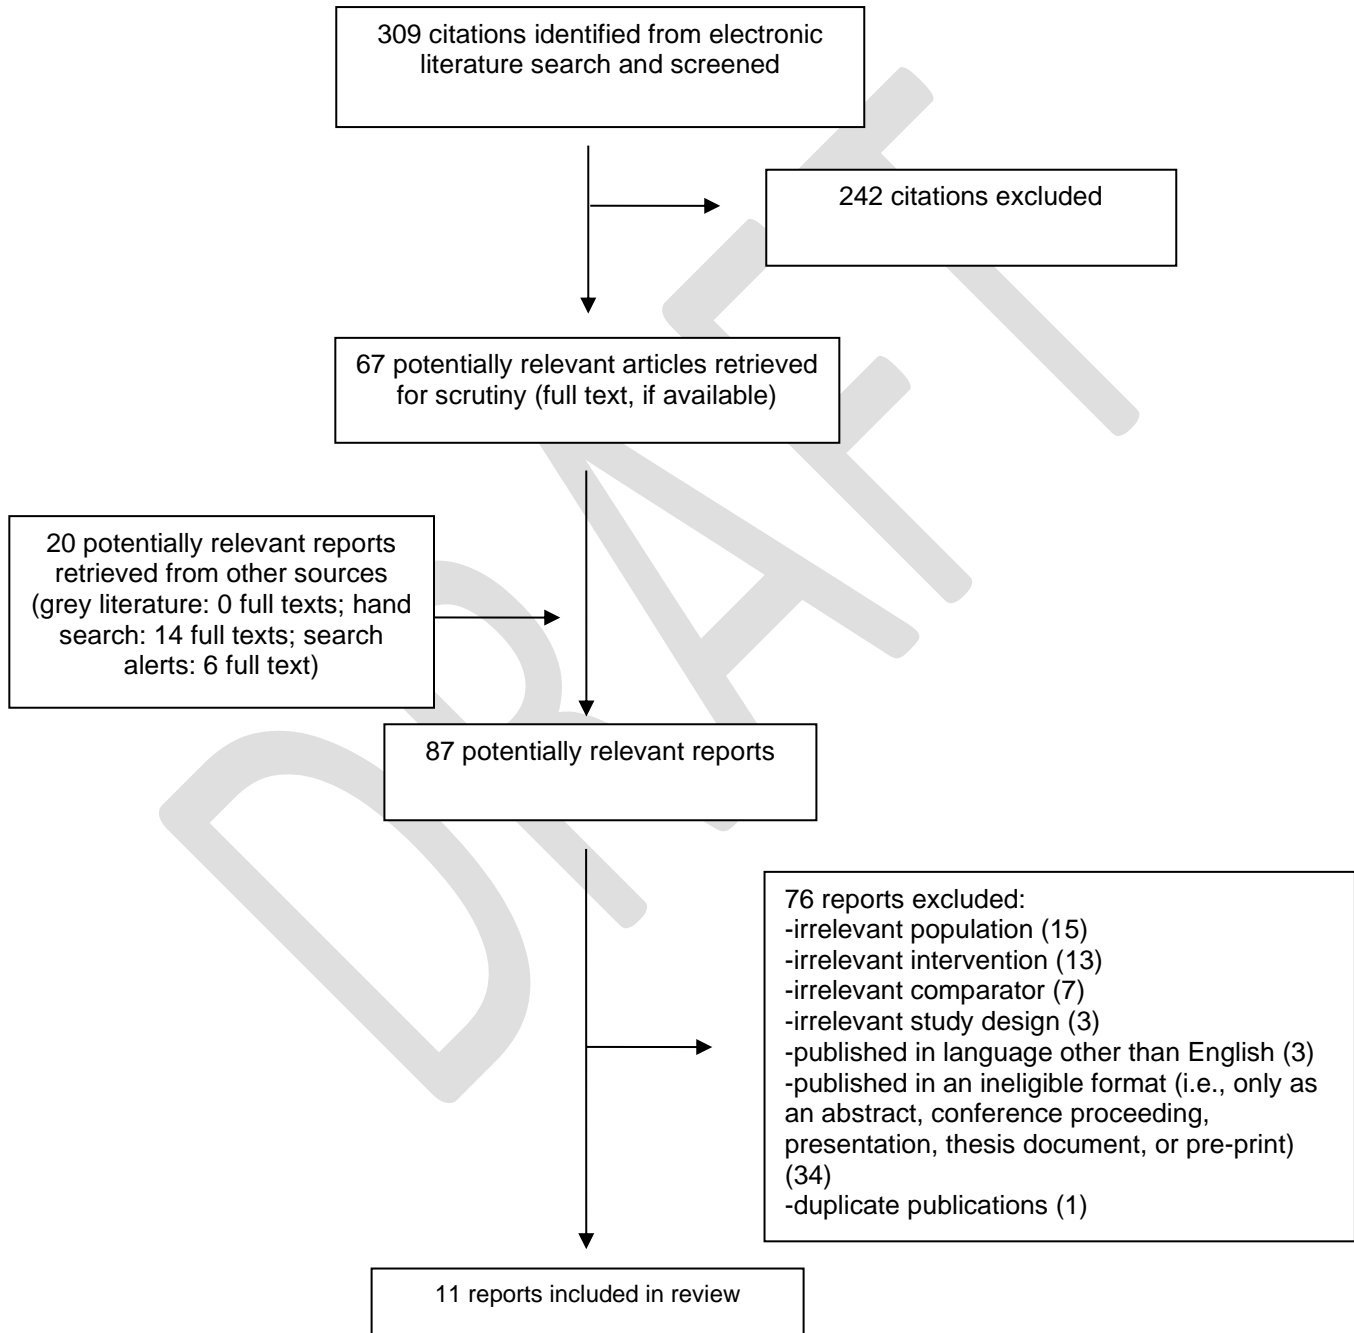



List of Included Publications

The citations provided in this list are the publications that were included in this rapid review (in reverse chronological and alphabetical order).

Delora A, Hadjialiakbari C, Percenti E, Torres J, Alderazi YJ, Ezzeldin R, Hassan AE, Ezzeldin M. Viz LVO versus Rapid LVO in detection of large vessel occlusion on CT angiography for acute stroke. *J Neurointerv Surg.* 2024 May 21;16(6):599-602. doi: 10.1136/jnis-2023-020445. PMID: 37355255.

Slater LA, Ravintharan N, Goergen S, et al. RapidAI compared with Human Readers of Acute Stroke Imaging for Detection of Intracranial Vessel Occlusion. *Stroke: Vascular and Interventional Neurology.* 2024;4:e001145

Chan N, Sibtain N, Booth T, de Souza P, Bibby S, Mah YH, Teo J, U-King-Im JM. Machine-learning algorithm in acute stroke: real-world experience. *Clin Radiol.* 2023 Feb;78(2):e45-e51. doi: 10.1016/j.crad.2022.10.007. Epub 2022 Nov 18. PMID: 36411087.

Soun JE, Zolyan A, McLouth J, et al. Impact of an automated large vessel occlusion detection tool on clinical workflow and patient outcomes. *Frontiers in neurology [electronic resource].* 2023; 14():1179250. PubMed: 37305764

Yedavalli V, Heit JJ, Dehkharghani S, et al. Performance of RAPID noncontrast CT stroke platform in large vessel occlusion and intracranial hemorrhage detection. *Front Neurol.* 2023; 14():. PubMed:

Mallon DH, Taylor EJR, Vittay OI, Sheeka A, Doig D, Lobotesis K. Comparison of automated ASPECTS, large vessel occlusion detection and CTP analysis provided by Brainomix and RapidAI in patients with suspected ischaemic stroke. *J Stroke Cerebrovasc Dis.* Oct 2022; 31(10):106702. PubMed: 35994882

Eldaya RW, Kansagra AP, Zei M, et al. Performance of Automated RAPID Intracranial Hemorrhage Detection in Real-World Practice: A Single-Institution Experience. *J Comput Assisted Tomogr.* Sep-Oct 01 2022; 46(5):770-774. PubMed: 35617649

Schlossman J, Ro D, Salehi S, Chow D, Yu W, Chang PD, Soun JE. Head-to-head comparison of commercial artificial intelligence solutions for detection of large vessel occlusion at a comprehensive stroke center. *Front Neurol.* 2022 Oct 10;13:1026609. doi: 10.3389/fneur.2022.1026609. PMID: 36299266; PMCID: PMC9588973.

Adhya J, Li C, Eisenmenger L, Cerejo R, Tayal A, Goldberg M, Chang W. Positive predictive value and stroke workflow outcomes using automated vessel density (RAPID-CTA) in stroke patients: One year experience. *Neuroradiol J.* 2021 Oct;34(5):476-481. doi: 10.1177/19714009211012353. Epub 2021 Apr 28. PMID: 33906499; PMCID: PMC8559016.

Dehkharghani S, Lansberg M, Venkatsubramanian C, Cereda C, Lima F, Coelho H, Rocha F, Qureshi A, Haerian H, Mont'Alverne F, Copeland K, Heit J. High-Performance Automated Anterior Circulation CT Angiographic Clot Detection in Acute Stroke: A Multireader Comparison. *Radiology.* 2021 Mar;298(3):665-670. doi: 10.1148/radiol.2021202734. Epub 2021 Jan 12. PMID: 33434110.

Amukotuwa SA, Straka M, Smith H, Chandra RV, Dehkharghani S, Fischbein NJ, Bammer R. Automated Detection of Intracranial Large Vessel Occlusions on Computed Tomography Angiography: A Single Center Experience. *Stroke.* 2019 Oct;50(10):2790-2798. doi: 10.1161/STROKEAHA.119.026259. Epub 2019 Sep 9. PMID: 31495328.

List of Excluded Publications and Reasons for Exclusion

The citations provided in this list are studies that were excluded after full-text review as part of the rapid review (in reverse chronological and alphabetical order).

Ineligible Population (n = 15):

- Alwood BT, Meyer DM, Ionita C, et al. Multicenter comparison using two AI stroke CT perfusion software packages for determining thrombectomy eligibility. *J Stroke Cerebrovasc Dis.* 2024 Jul;33(7):107750. Epub 2024 May 2. PubMed: 38703875.
- Pisani L, Haussen DC, Mohammaden M, et al. Comparison of CT Perfusion Software Packages for Thrombectomy Eligibility. *Ann Neurol.* 11 2023; 94(5):848-855. PubMed: 37584452
- Yedavalli V, Hamam O, Mohseni A, et al. Pretreatment brain CT perfusion thresholds for predicting final infarct volume in distal medium vessel occlusions. *J Neuroimaging.* Nov-Dec 2023; 33(6):968-975. PubMed: 37357133
- Xiong Y, Luo Y, Wang M, et al. Evaluation of Diffusion-Perfusion Mismatch in Acute Ischemic Stroke with a New Automated Perfusion-Weighted Imaging Software: A Retrospective Study. *Neurol.* Dec 2022; 11(4):1777-1788. PubMed: 36201112
- Wouters A, Robben D, Christensen S, et al. Prediction of Stroke Infarct Growth Rates by Baseline Perfusion Imaging. *Stroke.* 02 2022; 53(2):569-577. PubMed: 34587794
- Bousslama M, Ravindran K, Harston G, et al. Noncontrast Computed Tomography e-Stroke Infarct Volume Is Similar to RAPID Computed Tomography Perfusion in Estimating Postreperfusion Infarct Volumes. *Stroke.* 01 2021; 52(2):634-641. PubMed: 33430633
- Maegerlein C, Fischer J, Monch S, et al. Automated Calculation of the Alberta Stroke Program Early CT Score: Feasibility and Reliability. *Radiology.* 04 2019; 291(1):141-148. PubMed: 30720400
- Demeestere J, Scheldeman L, Cornelissen SA, et al. Alberta Stroke Program Early CT Score Versus Computed Tomographic Perfusion to Predict Functional Outcome After Successful Reperfusion in Acute Ischemic Stroke. *Stroke.* 10 2018; 49(10):2361-2367. PubMed: 30355098
- Automated CT perfusion imaging to aid in the selection of patients with acute ischemic stroke for mechanical thrombectomy: A health technology assessment. *Ont Health Technol Assess Ser.* 2020; 20(13):1-87. PubMed: 2005424949
- Lakatos L, Bolognese M, Müller M, Österreich M, von Hessling A. Automated Supra- and Infratentorial Brain Infarct Volume Estimation on Diffusion Weighted Imaging Using the RAPID Software. *Front Neurol.* 2022; 13():. PubMed:
- Kurmann CC, Kaesmacher J, Cooke DL, et al. Evaluation of time-resolved whole brain flat panel detector perfusion imaging using RAPID ANGIO in patients with acute stroke: Comparison with CT perfusion imaging. *J Neurointerv Surg.* 2023; 15(4):387-392. PubMed:
- Pistocchi S, Strambo D, Bartolini B, et al. MRI software for diffusion-perfusion mismatch analysis may impact on patients' selection and clinical outcome. *Eur Radiol.* 2022; 32(2):1144-1153. PubMed:
- Amukotuwa SA, Straka M, Dehkharghani S, Bammer R. Fast Automatic Detection of Large Vessel Occlusions on CT Angiography. *Stroke.* 2019 Dec;50(12):3431-3438. doi: 10.1161/STROKEAHA.119.027076. Epub 2019 Nov 4. PMID: 31679501; PMCID: PMC6878187.
- Albers GW, Wald MJ, Mlynash M, Endres J, Bammer R, Straka M, Maier A, Hinson HE, Sheth KN, Taylor Kimberly W, Molyneux BJ. Automated Calculation of Alberta Stroke Program Early CT Score: Validation in Patients With Large Hemispheric Infarct. *Stroke.* 2019 Nov;50(11):3277-3279. doi: 10.1161/STROKEAHA.119.026430. Epub 2019 Sep 10. PMID: 31500555.
- Siegler JE, Olsen A, Pulst-Korenberg J, Cristancho D, Rosenberg J, Raab L, Cucchiara B, Messé SR. Multicenter Volumetric Assessment of Artifactual Hypoperfusion Patterns using Automated CT Perfusion Imaging. *J Neuroimaging.* 2019 Sep;29(5):573-579. doi: 10.1111/jon.12641. Epub 2019 Jun 14. PMID: 31199025; PMCID: PMC6731139.

Ineligible Intervention (n = 13):

- Westwood M, Ramaekers B, Grimm S, Armstrong N, Wijnen B, Ahmadu C, de Kock S, Noake C, Joore M. Software with artificial intelligence-derived algorithms for analysing CT brain scans in people with a suspected acute stroke: a systematic review and cost-effectiveness analysis. *Health Technol Assess.* 2024 Mar;28(11):1-204. doi: 10.3310/RDPA1487. PMID: 38512017; PMCID: PMC11017149.



Yedavalli V, Kihira S, Shahrouki P, Hamam O, Tavakkol E, McArthur M, Qiao J, Johanna F, Doshi A, Vagal A, Khatri P, Srinivasan A, Chaudhary N, Bahr-Hosseini M, Colby GP, Nour M, Jahan R, Duckwiler G, Arnold C, Saver JL, Mocco J, Liebeskind DS, Nael K. CTP-based estimated ischemic core: A comparative multicenter study between Olea and RAPID software. *J Stroke Cerebrovasc Dis.* 2023 Nov;32(11):107297. doi: 10.1016/j.jstrokecerebrovasdis.2023.107297. Epub 2023 Sep 20. PMID: 37738915.

Werdiger F, Gotla S, Visser M, et al. Automated occlusion detection for the diagnosis of acute ischemic stroke: A detailed performance review. *Eur J Radiol.* Jul 2023; 164():110845. PubMed: 37148842

Lee KY, Liu CC, Chen DY, Weng CL, Chiu HW, Chiang CH. Automatic detection and vascular territory classification of hyperacute staged ischemic stroke on diffusion weighted image using convolutional neural networks. *Sci Rep.* 01 09 2023; 13(1):404. PubMed: 36624122

Al-Kawaz M, Primiani C, Urrutia V, Hui F. Impact of RapidAI mobile application on treatment times in patients with large vessel occlusion. *J Neurointerv Surg.* Mar 2022; 14(3):233-236. PubMed: 33795483

Sreekrishnan, Anirudh & Giurgiutiu, Dan-Victor & Kitamura, Felipe & Martinelli, Carlos & Abdala, Nitamar & Haerian, Hafez & Dehkharghani, Seena & Kwok, Keith & Yedavalli, Vivek & Heit, Jeremy. (2023). Decreasing false-positive detection of intracranial hemorrhage (ICH) using RAPID ICH 3. *Journal of stroke and cerebrovascular diseases : the official journal of National Stroke Association.* 32. 107396. 10.1016/j.jstrokecerebrovasdis.2023.107396.

Heit JJ, Coelho H, Lima FO, Granja M, Aghaebrahim A, Hanel R, Kwok K, Haerian H, Cereda CW, Venkatasubramanian C, Dehkharghani S, Carbonera LA, Wiener J, Copeland K, Mont'Alverne F. Automated Cerebral Hemorrhage Detection Using RAPID. *AJNR Am J Neuroradiol.* 2021 Jan;42(2):273-278. doi: 10.3174/ajnr.A6926. Epub 2020 Dec 24. PMID: 33361378; PMCID: PMC7872180.

Hokkinen L, Makela T, Savolainen S, Kangasniemi M. Computed tomography angiography-based deep learning method for treatment selection and infarct volume prediction in anterior cerebral circulation large vessel occlusion. *Acta Radiol Open.* Nov 2021; 10(11):20584601211060347. PubMed: 34868662

Hokkinen L, Makela T, Savolainen S, Kangasniemi M. Evaluation of a CTA-based convolutional neural network for infarct volume prediction in anterior cerebral circulation ischaemic stroke. *Eur Radiol Exp.* 06 24 2021; 5(1):25. PubMed: 34164743

Kim YC, Lee JE, Yu I, et al. Evaluation of Diffusion Lesion Volume Measurements in Acute Ischemic Stroke Using Encoder-Decoder Convolutional Network. *Stroke.* 06 2019; 50(6):1444-1451. PubMed: 31092169

Deshpande A, Elliott J, Jiang B, et al. End to end stroke triage using cerebrovascular morphology and machine learning. *Front Neurol.* 2023; 14(no pagination):. PubMed: 2026464700

Rajendra Acharya U, Meiburger KM, Faust O, et al. Automatic detection of ischemic stroke using higher order spectra features in brain MRI images. *Cogn Syst Res.* December 2019; 58():134-142. PubMed: 2002100357

Xiong Y, Huang CC, Fisher M, Hackney DB, Bhadelia RA, Selim MH. Comparison of Automated CT Perfusion Softwares in Evaluation of Acute Ischemic Stroke. *J Stroke Cerebrovasc Dis.* 2019 Dec;28(12):104392. doi: 10.1016/j.jstrokecerebrovasdis.2019.104392. Epub 2019 Sep 25. PMID: 31562038.

Ineligible Comparator (n = 7):

Siegler JE, Rosenberg J, Cristancho D, et al. Computed tomography perfusion in stroke mimics. *Int J Stroke.* 04 2020; 15(3):299-307. PubMed: 31409213

Kauw F, Heit JJ, Martin BW, van Ommen F, Kappelle LJ, Velthuis BK, de Jong HWAM, Dankbaar JW, Wintermark M. Computed Tomography Perfusion Data for Acute Ischemic Stroke Evaluation Using Rapid Software: Pitfalls of Automated Postprocessing. *J Comput Assist Tomogr.* 2020 Jan/Feb;44(1):75-77. doi: 10.1097/RCT.0000000000000946. PMID: 31804241.

Bulwa Z, Dasenbrock H, Osteraas N, Cherian L, Crowley RW, Chen M. Incidence of Unreliable Automated Computed Tomography Perfusion Maps. *J Stroke Cerebrovasc Dis.* Dec 2019; 28(12):104471. PubMed: 31680033

Campbell BC, Yassi N, Ma H, et al. Imaging selection in ischemic stroke: feasibility of automated CT-perfusion analysis. *Int J Stroke.* Jan 2015; 10(1):51-4. PubMed: 25319251

Hoving JW, Marquering HA, Majoie CBLM, et al. Volumetric and spatial accuracy of computed tomography perfusion estimated ischemic core volume in patients with acute ischemic stroke. *Stroke.* 2018; 49(10):2368-2375. PubMed: 627080929

Campbell BC, Yassi N, Ma H, et al. Imaging selection in ischemic stroke trials - Feasibility of automated CT perfusion analysis. *Cerebrovasc Dis.* May 2014; 37(Supplement 1):81. PubMed: 614324511



John S, Hussain SI, Piechowski B, Dogar MA. Discrepancy in core infarct between non-contrast CT and CT perfusion when selecting for mechanical thrombectomy. *J Cerebrovasc Endovasc Neurosurg.* 2020; 22(1):8-14. PubMed:

Ineligible Study Design (n = 3):

Gilotra K, Swarna S, Mani R, Basem J, Dashti R. Role of artificial intelligence and machine learning in the diagnosis of cerebrovascular disease. *Front Hum Neurosci.* 2023; 17():1254417. PubMed: 37746051

Morelli N, Colombi D, Michieletti E. Ischemic Core Estimation by CT Perfusion: A Matter of (rCBF) Numbers. *Am J Roentgenol.* 2023;221(2):284. <https://www.ncbi.nlm.nih.gov/pmc/articles/37134207>

Byrne D, Walsh JP, MacMahon PJ. An acute stroke CT imaging algorithm incorporating automated perfusion analysis. *Emerg. Jun 2019; 26(3):319-329.* PubMed: 30706257

Not Published in English (n = 3):

Cirio JJ, Diluca P, Ciardi C, et al. [Impact of artificial intelligence on therapeutic metrics of cerebrovascular attack during the COVID-19 pandemic]. *Medicina (B Aires).* 2023; 83(5):705-718. PubMed: 37870328

Cirio JJ, Diluca P, Ciardi C, et al. Impact of artificial intelligence on therapeutic metrics of cerebrovascular attack during the COVID-19 pandemic. *Medicina (Argentina).* 2023; 83(5):705-718

Cirio JJ, Ciardi C, Buezas M, et al. Implementation of artificial intelligence in hyperacute arterial reperfusion treatment in a comprehensive stroke center. *Neurologia Argentina.* 01 Oct 2021; 13(4):212-220.

Published in an Ineligible Format (n = 34):

Granja MF, Ramirez K, Espinel L, et al. Performance of RapidAI NCCT Stroke Software in Colombia's Early Stroke System: Preliminary Results. *Stroke Conference: American Stroke Association's.* 2024;55(Supplement 1).

Kashyap B, Herrmann AA, Droegemueller CJ, et al. Application of a Horizontal Communication Process in Combination With Artificial Intelligence (AI) to Improve Stroke Care in Patients With Large Vessel Occlusion (LVO). *Stroke Conference: American Stroke Association's.* 2024;55(Supplement 1).

Lavados P, Gonzalez P, Olavarria V, Albers GW. Improved Outcomes for Acute Ischemic Stroke Patients After Implementation of the RapidAI Platform in a Comprehensive Stroke Center in Santiago, Chile. *Stroke Conference: American Stroke Association's.* 2024;55(Supplement 1).

Mahdi Sowlat M, Zamarud A, Albers GW, Campbell B, Heit JJ, Spiotta AM. Detecting Medium Vessel Occlusions and Collateral Assessment With Multimodality AI Approach. *Stroke Conference: American Stroke Association's.* 2024;55(Supplement 1).

Malisch TW, Asif K, Geraghty S, Olges M, Copeland K, Albers G. Improved Stroke Outcomes Following Implementation of RapidAI Platform at Ascension-Illinois. *Stroke Conference: American Stroke Association's.* 2024;55(Supplement 1).

Yedavalli V, Heit JJ, Dehkharghani S, et al. Performance of RAPID noncontrast CT stroke platform in large vessel occlusion and intracranial hemorrhage detection. *medRxiv.* 2023; 16():. PubMed: 2026945999

Deshpande A, Elliott J, Jiang B, et al. End to end stroke triage using cerebrovascular morphology and machine learning. *medRxiv.* 2023; 01():. PubMed: 2023736914

Kroon L, Schutte C. Bridging the Gap: Telestroke's Impact on Access to Stroke Care in South Africa. *Int J Stroke.* October 2023; 18(3 Supplement):453. PubMed: 642828378

Almajidi M, Omairi M, Ajamaya B, Jevtic I, Antulov R. IMPLEMENTATION of AUTOMATED QUANTIFIED CTP in PATIENTS with NIHSS =6-A SINGLECENTER EXPERIENCE. *Neuroradiology.* September 2023; 65(Supplement 1):S98-S99. PubMed: 642678904

Biswas V, Sitaram A, Pollard C, Izzath MWK, Muir K. Variable penumbra but not core volume by occlusion site in large vessel occlusion. *Eur Stroke J.* May 2023; 8(2 Supplement):527-528. PubMed: 641735590

Kihira S, Shahrouki P, Tavakol E, et al. CTP-based estimated Ischemic Core: A Comparative Multicenter Study between Olea and RAPID software. *Eur Stroke J.* May 2023; 8(2 Supplement):525-526. PubMed: 641735460

Miao K, Miao J. Diagnosis and Prognosis of Stroke Using Artificial Intelligence and Imaging. *Neurology Conference: American Academy Of Neurology Annual Meeting, AAN.* 2023; 100(17 Supplement 2):. PubMed: 641672041

Affeldt ZS, Sabayan B, Droegemueller CJ, et al. Use of an Integrated Communication Tool Improves Stroke Care for Patients With Large Vessel Occlusion. *Acad Emerg Med.* May 2023; 30(Supplement 1):94. PubMed: 641605611



- Marigold R. Benefits of a regional CT artificial intelligence work stream in identifying patients for transfer to a comprehensive stroke centre (CSC) for mechanical thrombectomy. *Int J Stroke*. January 2023; 18(1 Supplement):26. PubMed: 640506051
- Leer M, McParland S, Wiggam I. How useful is artificial intelligence to support interpretation of CTA in hyperacute stroke?. *Int J Stroke*. January 2023; 18(1 Supplement):68-69. PubMed: 640505744
- Degan D, Turinese E, Iannucci G, et al. Rapid Software Effectiveness in Selecting Patients with Acute Ischemic Stroke Eligible for Endovascular Mechanical Thrombectomy. *Neurol Sci*. December 2022; 43(Supplement 1):S359. PubMed: 639930188
- Lambert J, Dewachter B, Demeestere J, Demaerel P, Lemmens R. Automated Aspects Software to Assist in Clinical Decisioning for Mechanical Thrombectomy. *Neuroradiology*. September 2022; 64(Supplement 1):S31. PubMed: 639201234
- Fouarge E, Ciobanu C, Cornet O, et al. Evaluation of Perfusion Imaging in Late Window Thrombectomy in Everyday Clinical Practice : Results of a Prospective Registry from a Network of Belgian Hospitals. *Eur Stroke J*. May 2022; 7(1 SUPPL):262. PubMed: 638375599
- Chang W, Eisenmenger L, Cerejo R, Li C, Goldberg MF. Artificial intelligence for automated detection of intracranial hemorrhage (rapid ICH): Initial clinical experience. *Stroke Conference*. 2022; 53(SUPPL 1):. PubMed: 637367335
- Catapano J, Lee K, Desai S, Ducruet AF, Albuquerque FC, Jadhav AP. Number-needed-to-review: A novel metric to assess triage efficiency of large vessel occlusion detection systems. *Stroke Conference*. 2022; 53(SUPPL 1):. PubMed: 637365693
- Vargas J, Moorhead S, Chaudry M, Turner R, Turk A. A comparison of two automated CTP algorithms for estimation of core infarct. *J Neurointerv Surg*. August 2021; 13(SUPPL 1):A72. PubMed: 635846865
- Dehkharghani S, Lansberg MG, Venkatsubramanian C, et al. Rapid-Ivo for automated detection of intracranial large vessel occlusion in ct angiography of the brain. *Stroke Conference: American Stroke Association International Stroke Conference, ISC*. 2021; 52(SUPPL 1):. PubMed: 634989714
- Miao KH, Miao JH. Enhancing Pain Management and Rehabilitation Outcomes in Stroke Patients with Artificial Intelligence and Medical Imaging. *J Investig Med*. 2021 April;69(4):935. PubMed: PM641217957
- Pisani L, Mohammad M, Bouzlama M, et al. Comparison of three automated ct perfusion software packages for thrombectomy eligibility and final infarct volume prediction. *Stroke Conference: American Stroke Association International Stroke Conference, ISC*. 2021; 52(SUPPL 1):. PubMed: 634989474
- Seo K, Kim GS, Yun PH, Suh SH. An introduction of the rapid software increased the number of mechanical thrombectomy with favorable outcome in stroke patients. *Neuroradiology*. 2019; 61(1):S106. PubMed: 631878630
- Mehta S, Panezai S, Strauss S, et al. RAPIDTM based treatment algorithms lead to faster activation of neurointervention team and reduce recanalization times. *Neurology Conference: 71st Annual Meeting of the American Academy of Neurology, AAN*. 2019; 92(15 Supplement 1):. PubMed: 629239448
- Bouzlama M, Rodrigues G, Ravindran K, Haussen D, Frankel M, Nogueira R. Ct perfusion and e-aspects automated noncontract CT ischemic core volumes: Correlations and clinical outcome prediction. *Eur Stroke J*. May 2019; 4(Supplement 1):405. PubMed: 628560803
- Chen L, Hallett C, Fernandes C, et al. Automated multi-feature quantification of plain CT in acute stroke. *Eur Stroke J*. May 2019; 4(Supplement 1):432. PubMed: 628561132
- Austein F, Jurgensen N, Lindner T, Jansen O. Impact of diferent reconstruction algorithms and diferent slice thickness on automated stroke software tool to detect early ischemic changes. *Clin Neuroradiol*. September 2018; 28(Supplement 1):S88. PubMed: 624304752
- Demeestere J, Scheldeman L, Cornelissen S, et al. Conventional and Automated Aspects vs. Ct perfusion core volume to predict functional outcome in reperfused acute ischemic stroke patients undergoing endovascular therapy. *Stroke Conference: American Heart Association/American Stroke Association*. 2018; 49(Supplement 1):. PubMed: 621004873
- Karamchandani RR, Singh SJ, Rhoten JB, et al. Computed tomography perfusion core infarct measurement compared to diffusion-weighted magnetic resonance imaging in patients with revascularization of anterior circulation, large artery occlusions. *Stroke Conference: American Heart Association/American Stroke Association*. 2018; 49(Supplement 1):. PubMed: 621004425
- Paz D, Yagoda D, Wein T. Single Site performance of AI software for stroke detection and Triage. *medRxiv*. 2021; (:):2021.04.02.21253083. PubMed:



Pourmussa B, Gorovoy D. A retrospective analysis of the diagnostic performance of an FDA approved software for the detection of intracranial hemorrhage. medRxiv. 2023; ():2023.11.02.23297974. PubMed:

Kamal H, Abdelhamid N, Zhu L, Sarraj A. Does RAPID reduce groin puncture times in acute, ischaemic stroke? Presented at International Stroke Conference; 21–24 February 2017; Houston (TX). Stroke 2017;48(Suppl. 1):TP296.

Duplicate Publications (n = 1):

Hoving JW, Marquering HA, Majoie C, et al. Volumetric and Spatial Accuracy of Computed Tomography Perfusion Estimated Ischemic Core Volume in Patients With Acute Ischemic Stroke. Stroke. 2018 10;49(10):2368-2375. PubMed: PM30355095

DRAFT



Characteristics of Included Publications

Table 1: Characteristics of Included Cohort Studies

Study citation, country, funding source	Study design and period	Population characteristics ^a and setting	Intervention and comparator(s)	Relevant clinical outcomes, length of follow-up
Soun et al. (2023) ¹ United States Funding source: The Radiological Society of North America Research Scholar Grant	Retrospective non-concurrent cohort December 2019 to June 2020 (pre-Rapid LVO group) and December 2020 to June 2021 (post-Rapid LVO group)	Population: 760 patients presenting with suspected acute ischemic stroke who were imaged using CTA (with or without Rapid LVO) ^b Age, median (IQR): 75 (65 to 83) years vs. 71.5 (65 to 79) years Sex or gender: 55.2% vs. 45.2% female, other sexes or genders NR Race: African American (2.3% vs. 3.2%), Asian or Pacific Islander (32.6% vs. 38.7%), Hispanic (30.2% vs. 17.7%), white (30.2% vs. 40.3%), other or did not specify (4.7% vs. 0.0%) Ethnicity, culture, or language: NR SES: NR Disability status: NR Setting: A single comprehensive stroke centre in the US.	Intervention: Clinician interpretation of CTA imaging with Rapid LVO (Rapid 4.9) for the detection of M1 MCA and intracranial ICA LVO (i.e., post-Rapid LVO group) Comparator: Clinician interpretation of CTA imaging without Rapid LVO for the detection of M1 MCA and intracranial ICA LVO (i.e., pre-Rapid LVO group)	Radiology report turnaround time; time from door to image; time from door to intubation; time from door to needle (i.e., tPA therapy); time from door to puncture (i.e., thrombectomy); time from door to revascularization; stroke-related neurological deficit (NIHSS scores); disability (mRS scores); response to therapy (TICI grades) Follow-up: Until discharge (mean time NR)
Adhya et al. (2021) ² United States Funding source: No financial support was received for this work.	Retrospective non-concurrent cohort November 2018 to November 2019 (pre-Rapid CTA group) and November 2019 to November 2020 (post-Rapid CTA group)	Population: 146 patients who arrived at the emergency department for stroke or neurological deficit and were imaged using CTA (with or without Rapid CTA post-processing) and subsequently underwent mechanical thrombectomy. Age: NR Sex or gender: NR Race, ethnicity, culture, or language: NR SES: NR Disability status: NR Setting: A large multi-hospital network in the US with comprehensive stroke centres and 24-hour neurointerventional coverage	Intervention: Clinician interpretation of CTA imaging with Rapid CTA (version NR) post-processing for the detection of LVO ^c (i.e., post-Rapid CTA group) Comparator: Clinician interpretation of CTA imaging without Rapid CTA for the detection of LVO ^c	Disability (mRS scores); time from CTA to groin puncture (i.e., thrombectomy) Follow-up: 90 days



Study citation, country, funding source	Study design and period	Population characteristics ^a and setting	Intervention and comparator(s)	Relevant clinical outcomes, length of follow-up
			(i.e., pre-Rapid CTA group)	

CTA = computed tomography angiography; ICA = internal carotid artery; ICH = intracranial hemorrhage; IQR = interquartile range; LVO = large vessel occlusion; MCA = middle cerebral artery; mRS = modified Rankin Scale; NIHSS = National Institutes of Health Stroke Scale; NR = not reported; SES = socioeconomic status; TICI = Thrombolysis in Cerebral Infarction; tPA = tissue plasminogen activator.

^a Intervention group versus comparator group, respectively.

^b Baseline demographics were reported for patients who received acute therapies (i.e., tPA, thrombectomy, or both) and not the entire study population (n = 43 for post-Rapid LVO group; n = 62 for pre-Rapid LVO).

^c Unclear which types of LVO were considered eligible. The study population included patients with occlusions of the ICA, carotid terminus, M1 MCA segment, or M2 MCA segment.

Table 2: Characteristics of Included Diagnostic Accuracy Studies

Study citation, country, funding source	Study design and period	Target condition	Population characteristics and setting	Index test and reference standard	Relevant outcomes
LVO					
Delora et al. (2024) ³ United States Funding source: The authors did not declare a specific grant for this research from any funding agency. HCA Healthcare supported this research and had	Cross-sectional study with unclear selection January 2022 to January 2023	LVO ^a	Population: 360 patients who underwent CTA for suspected acute stroke Age, mean (SD): 65 (16.5) years Sex or gender: 44.4% males, other sexes or genders NR Race, ethnicity, culture, or language: NR SES: NR Disability status: NR Setting: Two community-based comprehensive stroke centers in the US	Index test: Evaluation of CTA by Rapid LVO (version 5.2.2) alone Reference standard: Interpretation of CTA by a single diagnostic or interventional neuroradiologist (with access to Rapid LVO results).	Sensitivity; specificity; TP; FP; TN; FN; PPV; NPV



Study citation, country, funding source	Study design and period	Target condition	Population characteristics and setting	Index test and reference standard	Relevant outcomes
financial interest in Viz.ai					
Slater et al. (2024) ⁴ Australia Funding source: No financial support was received for this work.	Cohort selected cross-sectional study April 2021 to August 2021	LVO (defined as occlusions of the intracranial ICA, M1 or M2 MCA segments, basilar artery, or intracranial vertebral artery)	Population: 500 adult patients (aged ≥ 18 years) with clinical suspicion of ischemic stroke who underwent multimodality imaging (i.e., NCCT of the brain, CTA of the head, and CT perfusion) with RapidAI interpretation Age, median (IQR): 70 (56 to 80) years Sex or gender: 49.6% men, other sexes or genders NR Race, ethnicity, culture, or language: NR SES: NR Disability status: NR Setting: A single comprehensive stroke centre in Australia	Index test: Rapid CTA (RapidAI 5.1) alone Reference standard: Independent assessment by 3 interventional neuroradiologists (with 10, 10, and 3 years of experience). Whenever the panel was not unanimous, a 4 th neurointerventional radiologist (with 13 years of experience) made an additional independent assessment and disagreements were reviewed until consensus was reached.	Sensitivity; specificity
Chan et al. (2023) ⁵ United Kingdom Funding source: The funding source for this study was unclear. The authors declared financial interests and relationships with industry and medical research granting agencies	Cohort selected cross-sectional study January 2021 to March 2021	Terminal ICA and M1 MCA LVO	Population: 104 consecutive patients with suspected acute stroke who underwent imaging CT or CTA imaging Age, median (range): 62 (19 to 93) years Sex or gender: 41.3% women, other sexes or genders NR Race, ethnicity, culture, or language: NR SES: NR Disability status: NR Setting: A single tertiary neuroscience institution in the UK	Index test: Evaluation of CTA by Rapid CTA (version NR) alone Reference standard: Consensus assessment of LVO on CTA by 2 experienced neuroradiologists blinded to the initial report and the Rapid CTA interpretation	Sensitivity; specificity; TP; FP; TN; FN; PPV; NPV
Soun et al. (2023) ¹ United States Funding source: The Radiological Society of North	Cohort selected cross-sectional study December 2020 to June 2021	M1 MCA and intracranial ICA LVO	Population: 321 patients presenting with suspected acute ischemic stroke who were imaged using CTA with Rapid LVO ^p Age, median (IQR): 75 (65 to 83) years Sex or gender: 55.2% female, other sexes or genders NR	Index test: Evaluation of CTA by Rapid LVO (Rapid 4.9) alone Reference standard: Assessment of LVO on CTA from the radiologist's reports (with Rapid LVO), which were verified by a board-certified neuroradiologist (with 9 years of experience). For complex cases where the	Sensitivity; specificity; PPV; NPV



Study citation, country, funding source	Study design and period	Target condition	Population characteristics and setting	Index test and reference standard	Relevant outcomes
America Research Scholar Grant			<p>Race: 2.3% African American, 32.6% Asian or Pacific Islander, 30.2% Hispanic, 30.2% white, 4.7% other or did not specify</p> <p>Ethnicity, culture, or language: NR</p> <p>SES: NR</p> <p>Disability status: NR</p> <p>Setting: A single comprehensive stroke centre in the US</p>	reference standard was not clearly delineated, 2 additional two additional neuroradiologists (with 9 and 11 years of experience) determined the reference standard	
Yedavalli et al. (2023) ⁶ United States Funding source: No financial support was received for this work	Cohort selected cross-sectional study Study period was NR	Distal intracranial ICA and M1 segment of the MCA	<p>Population: 244 patients with suspected stroke who underwent NCCT and CTA imaging</p> <p>Age, mean (SD): NR</p> <p>Sex or gender: NR</p> <p>Race, ethnicity, culture, or language: NR</p> <p>SES: NR</p> <p>Disability status: NR</p> <p>Setting: Patient data from 7 hospitals (including academic and community hospitals) and 2 research studies that enrolled acute LVO patients were included</p>	<p>Index test: Evaluation of NCCT by Rapid NCCT Stroke platform (using the Rapid HVS to detect LVO) alone</p> <p>Reference standard: Consensus assessment of LVO on CTA by 2 of 3 neuroradiologists</p>	Sensitivity; specificity; TP; FP; TN; FN.
Mallon et al. (2022) ⁷ United Kingdom Funding source: Imperial Health Charity and National Institute for Health Research Biomedical Research Centre based at Imperial College Healthcare NHS Trust and Imperial College London	Cohort selected cross-sectional study January 2016 and December 2020	LVO of the ICA and the M1 and M2 MCA segments	<p>Population: 90 patients undergoing evaluation with CT perfusion for suspected anterior circulation LVO^c</p> <p>Age, median (IQR): 70.5 (58 to 80) years</p> <p>Sex or gender: 48% female, 52% male, other sexes or genders NR</p> <p>Race, ethnicity, culture, or language: NR</p> <p>SES: NR</p> <p>Disability status: NR</p> <p>Setting: A single academic health science centre in the UK</p>	<p>Index test: Evaluation of CTA by RapidAI (version NR) alone</p> <p>Reference standard: Evaluation of CTA by a single neuroradiologist (with 4 years experience)</p>	Sensitivity; specificity; TP; FP; TN; FN; PPV; NPV

Study citation, country, funding source	Study design and period	Target condition	Population characteristics and setting	Index test and reference standard	Relevant outcomes
Schlossman et al. (2022) ⁸ United States Funding source: Canon Medical	Cohort selected cross-sectional study December 2020 to June 2021	M1 and M2 MCA and intracranial ICA LVO	Population: 263 patients who underwent CTA for suspected acute ischemic stroke Age, median (IQR): 68 (56 to 79) years Sex or gender: 46.4% female, other sexes or genders NR Race, ethnicity, culture, or language: NR SES: NR Disability status: NR Setting: A single comprehensive stroke centre in US	Index test: Evaluation of CTA by Rapid LVO (RapidAI 4.9) alone Reference standard: Consensus assessment of LVO on CTA by 2 board-certified neuroradiologists (with 9 and 10 years of experience), with a 3 rd board-certified neuroradiologist (with 11 years experience) to adjudicate disagreements	Sensitivity; specificity; TP; FP; TN; FN; PPV; NPV
Adhya et al. (2021) ² United States Funding source: No financial support was received for this work	Cohort selected cross-sectional study November 2019 to November 2020	LVO ^a	Population: 310 patients who underwent CTA imaging for the evaluation of suspected acute ischemic stroke or neurological deficit with relative vessel density of 60% or less Age, mean (SD): 70.0 (NR) years Sex or gender: 53% female, 47% male, other sexes or genders NR Race, ethnicity, culture, or language: NR SES: NR Disability status: NR Setting: A large multi-hospital network in the US with comprehensive stroke centres and 24-hour neurointerventional coverage	Index test: Evaluation of CTA by Rapid CTA (version NR) alone Reference standard: Consensus assessment of LVO on CTA by 2 board-certified neuroradiologists, with a 3 rd board-certified neuroradiologist to adjudicate disagreements (although not required as there were no disagreements)	Sensitivity; specificity; TP; FP; TN; FN; PPV; NPV (at < 45% and < 60% thresholds for relative vessel density)
Dehkharghani et al. (2021) ⁹ United States Funding source: The authors received support from iSchemaView and the National Institute of Neurologic Disorders and Stroke	Case-control selected cross-sectional study Study period was NR	M1 MCA and intracranial ICA LVO	Population: 217 patients who underwent CTA imaging for suspected acute ischemic stroke Age, mean (SD): 64 (16) years Sex or gender: 46% female, 54% male, 1% unknown, other sexes or genders NR Race, ethnicity, culture, or language: NR SES: NR Disability status: NR Setting: Patient data from recent cerebrovascular trials and institutional	Index test: Evaluation of CTA by Rapid LVO (version 1.0) alone Reference standard: Consensus assessment of LVO on CTA from up to 3 board-certified neuroradiologists with subspecialty certification (with 11, 7 and 7 years of experience)	Sensitivity; specificity; TP; FP; TN; FN

Study citation, country, funding source	Study design and period	Target condition	Population characteristics and setting	Index test and reference standard	Relevant outcomes
			registries from 11 worldwide sites were included		
Amukotuwa et al. (2019) ¹⁰ Australia Funding source: No financial support was received for this work.	Cohort selected cross-sectional study January 2017 to December 2018	LVO (defined as occlusions of the M1 MCA and intracranial ICA) and M2 MCA occlusions	Population: 477 patients who underwent multimodal brain CT (including NCCT, CT perfusion, and CTA) for suspected acute ischemic stroke. Age, median (IQR): 71 (60 to 80) years Sex or gender: 43.2% female, 56.8% male, other sexes or genders NR Race, ethnicity, culture, or language: NR SES: NR Disability status: NR Setting: A single regional hospital in Australia	Index test: Evaluation of CTA by Rapid CTA (RapidAI 4.9) alone. Reference standard: Consensus assessment of LVO on unenhanced CT, CTP, and CTA by 2 diagnostic neuroradiologists (with 8 and 9 years of post-fellowship experience), with a 3 rd interventional neuroradiologist (with 7 years of experience) to verify decisions.	Sensitivity; specificity; TP; FP; TN; FN; PPV; NPV; AUC
ICH					
Eldaya et al. (2022) ¹¹ United States Funding source: NR	Cohort selected cross-sectional study May 2020 to October 2020	ICH	Population: 308 patients presenting with acute neurological deficit suspicious for acute stroke and underwent NCCT imaging with Rapid ICH Age, mean (SD): 61.0 (16.7) years Sex or gender: NR Race, ethnicity, culture, or language: NR SES: NR Disability status: NR Setting: A single large, tertiary comprehensive stroke centre in the US	Index test: Evaluation of NCCT by a board certified or board-eligible neuroradiologist, typically in conjunction with a radiology trainee, using Rapid ICH (version NR) Reference standard: When standalone Rapid ICH and neuroradiologist interpretation were concordant, it was considered the reference standard. In cases where there was disagreement between Rapid ICH and neuroradiologist interpretation, the reference standard was a consensus panel of 3 board-certified neuroradiologists (with 3, 6, and 24 years of experience)	Sensitivity; specificity; TP; FP; TN; FN; PPV; NPV

AUC = area under the receiver operating characteristic curve; CT = computed tomography; CTA = computed tomography angiography; CTP = computed tomography perfusion; FN = false negatives; FP = false positives; ICA = internal carotid artery; MCA = middle cerebral artery; NCCT = non-contrast computed tomography; NPV = negative predictive value; NR = not reported; PPV = positive predictive value; SES = socioeconomic status; TN = true negatives; TP = true positives; tPA = tissue plasminogen activator.

^a Unclear which types of LVO were considered eligible. In Delora et al. (2024),³ the study population included patients with occlusions of the ICA, M1 MCA segment, and M2 MCA segment. The study population from Adhya et al. (2021) included patients with occlusions of the ICA, carotid terminus, M1 MCA segment, and M2 MCA segment.

^b Baseline demographics were reported for patients who received acute therapies (i.e., tPA, thrombectomy, or both; n = 48) and not the entire study population.

^c Baseline demographics were reported for patients with LVO according to the reference standard (n = 62) and not the entire study population.



Critical Appraisal of Included Studies

ROBINS-I Detailed Assessments

Table 3: Risk of Bias Assessment of Time to Intervention Outcomes Reported by Soun et al. (2023)¹ – ROBINS-I

Domain/question	Judgement	Comments
Decide whether to proceed with a risk-of-bias assessment		
0.1. Did the authors make any attempt to control for confounding?	No	There were no adjustments for confounding variables (e.g., age, sex or gender, race, ethnicity, disease severity, comorbidities, neurologist experience).
0.2. Is there sufficient potential for confounding that an unadjusted result should not be considered further?	Yes	Two cohorts of patients were enrolled during separate time periods. There were differences in patient disease characteristics at baseline and in the level of neurologist training between time periods which could affect the outcomes. This is particularly concerning as the study period partially overlapped with the COVID-19 pandemic, where many changes to the hospital system could have impacted time to treatment outcomes.
0.3. Was the method of measuring the outcome inappropriate?	NI	It was unclear who assessed time to intervention outcomes or how they were measured.
Risk of bias judgment	Critical (no further assessment is required)	For time to intervention outcomes, the study is at critical risk of bias due to confounding, as there were no attempts to control for differences across the 2 time periods which could have affected the outcomes.

NI = no information; ROBINS-I = Risk Of Bias In Nonrandomized Studies – of Interventions.



Table 4: Risk of Bias Assessment of Functional Status Outcomes Reported by Soun et al. (2023)¹ – ROBINS-I

Domain/question	Judgement	Comments
Decide whether to proceed with a risk-of-bias assessment		
0.1. Did the authors make any attempt to control for confounding?	Yes	For change in NIHSS score and NIHSS at discharge, there were adjustments for the effects of high cholesterol, heart disease, atrial fibrillation, therapies received, and NIHSS on admission. However, the authors provided no rationale for how these factors were selected, and it is unlikely that this would include all potential sources of baseline confounding. Additionally, there was no information as to how these confounding variables were measured. For the remaining measure of functional status, there were no adjustments for confounding variables.
0.2. Is there sufficient potential for confounding that an unadjusted result should not be considered further?	Yes	Two cohorts of patients were enrolled during separate time periods. There were differences in patient disease characteristics at baseline and in the level of neurologist training between time periods which could affect the outcomes. This is particularly concerning as the study period partially overlapped with the COVID-19 pandemic, where many changes to the hospital system could have impacted patient outcomes.
0.3. Was the method of measuring the outcome inappropriate?	Probably no	The tools used to assess outcomes related to functional status were reported, but it was unclear who conducted the assessments.
Risk of bias judgment	Critical (no further assessment is required)	For functional status outcomes, the study is at critical risk of bias due to confounding, as there were no or limited attempts to control for differences across the 2 time periods which could have affected the outcomes.

NIHSS = National Institutes of Health Stroke Scale; ROBINS-I = Risk Of Bias In Nonrandomized Studies – of Interventions.



Table 5: Risk of Bias Assessment of Response to Therapy Outcomes Reported by Soun et al. (2023)¹ – ROBINS-I

Domain/question	Judgement	Comments
Decide whether to proceed with a risk-of-bias assessment		
0.1. Did the authors make any attempt to control for confounding?	No	There were no adjustments for confounding variables (e.g., age, sex or gender, race, ethnicity, disease severity, comorbidities, neurologist experience)
0.2. Is there sufficient potential for confounding that an unadjusted result should not be considered further?	Yes	Two cohorts of patients were enrolled during separate time periods. There were differences in patient disease characteristics at baseline and in the level of neurologist training between time periods which could affect the outcomes. This is particularly concerning as the study period partially overlapped with the COVID-19 pandemic, where many changes to the hospital system could have impacted patient outcomes.
0.3. Was the method of measuring the outcome inappropriate?	Probably no	The tools used to assess response to treatment outcomes were reported, but it was unclear who conducted the assessments.
Risk of bias judgment	Critical (no further assessment is required)	For response to treatment outcomes, the study is at critical risk of bias due to confounding, as there were no attempts to control for differences across the 2 time periods which could have affected the outcomes.

ROBINS-I = Risk Of Bias In Nonrandomized Studies – of Interventions.



Table 6: Risk of Bias Assessment of Time to Intervention Outcomes Reported by Adhya et al. (2021)² – ROBINS-I

Domain/question	Judgement	Comments
Decide whether to proceed with a risk-of-bias assessment		
0.1. Did the authors make any attempt to control for confounding?	No	There were no adjustments for confounding variables (e.g., age, sex or gender, race, ethnicity, disease severity, comorbidities, neurologist experience)
0.2. Is there sufficient potential for confounding that an unadjusted result should not be considered further?	Yes	Two cohorts of patients were enrolled during separate time periods. There could have been differences in patient disease characteristics at baseline and in the level of neurologist training between time periods which could affect the outcomes but insufficient information was reported to inform about these differences. This is particularly concerning as the study period partially overlapped with the COVID-19 pandemic, where many changes to the hospital system could have impacted time to treatment outcomes.
0.3. Was the method of measuring the outcome inappropriate?	NI	It was unclear who assessed time to intervention outcomes or how they were measured.
Risk of bias judgment	Critical (no further assessment is required)	For time to intervention outcomes, the study is at critical risk of bias due to confounding, as there were no attempts to control for differences across the 2 time periods which could have affected the outcomes.

NI = no information; ROBINS-I = Risk Of Bias In Nonrandomized Studies – of Interventions.



Table 7: Risk of Bias Assessment of Functional Status Outcomes Reported by Adhya et al. (2021)² – ROBINS-I

Domain/question	Judgement	Comments
Decide whether to proceed with a risk-of-bias assessment		
0.1. Did the authors make any attempt to control for confounding?	No	There were no adjustments for confounding variables (e.g., age, sex or gender, race, ethnicity, disease severity, comorbidities, neurologist experience)
0.2. Is there sufficient potential for confounding that an unadjusted result should not be considered further?	Yes	Two cohorts of patients were enrolled during separate time periods. There could have been differences in patient disease characteristics at baseline and in the level of neurologist training between time periods which could affect the outcomes but insufficient information was reported to inform about these differences. This is particularly concerning as the study period partially overlapped with the COVID-19 pandemic, where many changes to the hospital system could have impacted patient outcomes.
0.3. Was the method of measuring the outcome inappropriate?	Probably no	The tools used to assess outcomes related to functional status were reported, but it was unclear who conducted the assessments.
Risk of bias judgment	Critical (no further assessment is required)	For functional status outcomes, the study is at critical risk of bias due to confounding, as there were no attempts to control for differences across the 2 time periods which could have affected the outcomes.

ROBINS-I = Risk Of Bias In Nonrandomized Studies – of Interventions.



QUADAS-2 Detailed Assessments

Table 8: Risk of Bias Assessment of Delora et al. (2024)³ – QUADAS-2

Domain/question	Judgement	Comments
Domain 1: Patient Selection		
A. Risk of Bias		
<ul style="list-style-type: none"> Was a consecutive or random sample of patients enrolled? 	Unclear	There is insufficient reporting of how the patient population was selected to determine if it was a consecutive or random sample.
<ul style="list-style-type: none"> Was a case-control design avoided? 	Unclear	The methods for patient selection were unclear.
<ul style="list-style-type: none"> Did the study avoid inappropriate exclusions? 	Unclear	The eligibility criteria were not reported. Some patients were excluded for missing data, but it was unclear which types of data were missing and for what reasons.
Risk of bias: Could the selection of patients have introduced bias?	Unclear	'Unclear' for all signalling questions.
B. Concerns regarding applicability		
Applicability: Is there concern that the included patients do not match the review question?	Low	Patients were those who underwent multimodal CT for suspected acute ischemic stroke, which is directly relevant to the review question.
Domain 2: Index Test		
A. Risk of Bias		
<ul style="list-style-type: none"> Were the index test results interpreted without knowledge of the results of the reference standard? 	Yes	The study examined the diagnostic performance of Rapid LVO alone (which did not have access to the results of the reference standard).
<ul style="list-style-type: none"> If a threshold was used, was it pre-specified? 	Unclear	The threshold of relative vessel density for detecting LVO was not described.
Risk of bias: Could the conduct or interpretation of the index test have introduced bias?	Unclear	There is insufficient information to determine whether the threshold of relative vessel density for detecting LVO was pre-specified.
B. Concerns regarding applicability		
Applicability: Is there concern that the index test, its conduct, or interpretation differ from the review question?	High	The index test was evaluation of CTA by Rapid LVO alone, which is different from our primary review question and how the tool is used in practice (i.e., Rapid LVO alongside clinician interpretation).
Domain 3: Reference Standard		
A. Risk of Bias		

Domain/question	Judgement	Comments
<ul style="list-style-type: none"> Is the reference standard likely to correctly classify the target condition? 	Yes	The reference standard diagnosis was interpretation of CTA by a single diagnostic or interventional neuroradiologist (with access to Rapid LVO results).
<ul style="list-style-type: none"> Were the reference standard results interpreted without knowledge of the results of the index test? 	No	The reference standard results were interpreted with knowledge of the analysis by Rapid LVO and Viz LVO (2 automated LVO detection software that were running simultaneously).
Risk of bias: Could the reference standard, its conduct, or its interpretation have introduced bias?	High	Knowledge of the index test results could have influenced the interpretation of the reference standard, which may bias estimates of agreement between the index test and the reference standard results.
B. Concerns regarding applicability		
Applicability: Is there concern that the target condition as defined by the reference standard does not match the review question?	Low	The target condition was LVO (i.e., ischemic stroke), and was likely to be correctly classified by the reference standard, which is directly relevant to the review question.
Domain 4: Flow and Timing		
A. Risk of Bias		
<ul style="list-style-type: none"> Was there an appropriate interval between index test(s) and reference standard? 	NA	Not applicable. The index test and the reference standard used the same CT images, and the timing of interpretation is not relevant.
<ul style="list-style-type: none"> Did all patients receive a reference standard? 	Yes	There were no indications that all patients did not receive a reference standard.
<ul style="list-style-type: none"> Did patients receive the same reference standard? 	Yes	All patients received the same reference standard.
<ul style="list-style-type: none"> Were all patients included in the analysis? 	Yes	All 360 patients were included in the Rapid LVO confusion matrix and the calculation of diagnostic parameters.
Risk of bias: Could the patient flow have introduced bias?	Low	'Yes' or 'NA' for all signalling questions.

CT = computed tomography; CTA = computed tomography angiography; LVO = large vessel occlusion; NA = not applicable; QUADAS-2 = Quality Assessment of Diagnostic Accuracy Studies 2.



Table 9: Risk of Bias Assessment of Slater et al. (2024)⁴ – QUADAS-2

Domain/question	Judgement	Comments
Domain 1: Patient Selection		
A. Risk of Bias		
<ul style="list-style-type: none"> Was a consecutive or random sample of patients enrolled? 	Yes	Patients who presented to a single comprehensive stroke center over a 5-month interval with clinical suspicion of ischemic stroke and who underwent multimodality imaging with RapidAI interpretation were included. From this cohort, patients were excluded if they had incomplete imaging or if CT angiography was of inadequate quality (e.g., those with poor contrast bolus injection or patient motion artifact). Although not explicitly reported, it appears likely that all eligible patients were included.
<ul style="list-style-type: none"> Was a case-control design avoided? 	Yes	Patient selection was independent of the results of the reference standard.
<ul style="list-style-type: none"> Did the study avoid inappropriate exclusions? 	Yes	Although the study excluded patients with inadequate image quality, this is likely aligned with how the test would be used in practice.
Risk of bias: Could the selection of patients have introduced bias?	Low	'Yes' for all signalling questions.
B. Concerns regarding applicability		
Applicability: Is there concern that the included patients do not match the review question?	Low	Patients with clinical suspicion of ischemic stroke, which is directly relevant to the review question.
Domain 2: Index Test		
A. Risk of Bias		
<ul style="list-style-type: none"> Were the index test results interpreted without knowledge of the results of the reference standard? 	Yes	The study examined the diagnostic performance of RapidAI alone (which did not have access to the results of the reference standard).
<ul style="list-style-type: none"> If a threshold was used, was it pre-specified? 	Yes	<p>"We did not calculate the area under the receiver operating curve for RapidAI detection of arterial occlusion. The test has only 1 threshold, and receiver operating curves are better suited to perform in diagnostic tests with multiple thresholds" (p. 7).⁴</p> <p>The authors indicated that RapidAI only has 1 threshold, so they likely used the threshold specified by the manufacturer of the test.</p>
Risk of bias: Could the conduct or interpretation of the index test have introduced bias?	Low	'Yes' for all signalling questions.
B. Concerns regarding applicability		
Applicability: Is there concern that the index test, its conduct, or interpretation differ from the review question?	High	The index test was evaluation of CTA by RapidAI CTA module alone, which is different from our primary review question and how the tool is used in practice (i.e., Rapid CTA alongside clinician interpretation).

Domain/question	Judgement	Comments
Domain 3: Reference Standard		
A. Risk of Bias		
<ul style="list-style-type: none"> Is the reference standard likely to correctly classify the target condition? 	Yes	The reference standard diagnosis was made by a panel of 4 interventional neuroradiologists (with access to Rapid LVO results).
<ul style="list-style-type: none"> Were the reference standard results interpreted without knowledge of the results of the index test? 	Unclear	<p>“Three interventional neuroradiologists [...] independently assessed all studies to determine the presence and site of arterial occlusions. Whenever this panel was not unanimous, a fourth neurointerventional radiologist [...] made an additional independent assessment, and disagreements were reviewed. A consensus diagnosis was obtained for all cases” (p. 4).⁴</p> <p>It was not explicitly stated whether the reference standard assessments were conducted without knowledge of the index test results.</p>
Risk of bias: Could the reference standard, its conduct, or its interpretation have introduced bias?	Unclear	Unclear if the neuroradiologists had knowledge of the results of the index test.
B. Concerns regarding applicability		
Applicability: Is there concern that the target condition as defined by the reference standard does not match the review question?	Low	The target condition was LVO (i.e., ischemic stroke), and was likely to be correctly classified by the reference standard, which is directly relevant to the review question.
Domain 4: Flow and Timing		
A. Risk of Bias		
<ul style="list-style-type: none"> Was there an appropriate interval between index test(s) and reference standard? 	NA	Not applicable. The index test and the reference standard used the same CT images, and the timing of interpretation is not relevant.
<ul style="list-style-type: none"> Did all patients receive a reference standard? 	Yes	All 500 included patients were assessed by the reference standard (and a consensus diagnosis was obtained for each).
<ul style="list-style-type: none"> Did patients receive the same reference standard? 	Yes	The reference standard was consistent for all patients.
<ul style="list-style-type: none"> Were all patients included in the analysis? 	Yes	There were no indications to suggest that all patients were not included in the analysis.
Risk of bias: Could the patient flow have introduced bias?	Low	‘Yes’ or ‘NA’ for all signalling questions.

CT = computed tomography; CTA = computed tomography angiography; LVO = large vessel occlusion; NA = not applicable; QUADAS-2 = Quality Assessment of Diagnostic Accuracy Studies 2.

Table 10: Risk of Bias Assessment of Chan et al. (2023)⁵ – QUADAS-2

Domain/question	Judgement	Comments
Domain 1: Patient Selection		
A. Risk of Bias		
<ul style="list-style-type: none"> Was a consecutive or random sample of patients enrolled? 	Yes	“The CT and CTA images performed to exclude stroke for 104 consecutive adult patients presenting from January to March 2021 at a single tertiary neuroscience institution were analysed” (p. e46). ⁵
<ul style="list-style-type: none"> Was a case-control design avoided? 	Yes	Consecutive patients presenting with suspected acute stroke were included. Patient selection was independent of the results of the reference standard.
<ul style="list-style-type: none"> Did the study avoid inappropriate exclusions? 	Yes	Only 2/104 patients were excluded at the time of enrollment. The rationale for exclusions were provided and reasonable.
Risk of bias: Could the selection of patients have introduced bias?	Low	‘Yes’ for all signalling questions.
B. Concerns regarding applicability		
Applicability: Is there concern that the included patients do not match the review question?	Low	Patients were those who were being assessed for possible acute stroke, which is directly relevant to the review question.
Domain 2: Index Test		
A. Risk of Bias		
<ul style="list-style-type: none"> Were the index test results interpreted without knowledge of the results of the reference standard? 	Yes	The study examined the diagnostic performance of Rapid CTA alone (which did not have access to the results of the reference standard).
<ul style="list-style-type: none"> If a threshold was used, was it pre-specified? 	Unclear	The threshold of relative vessel density for detecting LVO was not described.
Risk of bias: Could the conduct or interpretation of the index test have introduced bias?	Unclear	There is insufficient information to determine whether the threshold of relative vessel density for detecting LVO was pre-specified.
B. Concerns regarding applicability		
Applicability: Is there concern that the index test, its conduct, or interpretation differ from the review question?	High	The index test was evaluation of CTA by Rapid CTA alone, which is different from our primary review question and how the tool is used in practice (i.e., Rapid CTA alongside clinician interpretation).
Domain 3: Reference Standard		
A. Risk of Bias		
<ul style="list-style-type: none"> Is the reference standard likely to correctly classify the target condition? 	Yes	The reference standard diagnosis was determined by consensus among 2 experienced neuroradiologists.

Domain/question	Judgement	Comments
<ul style="list-style-type: none"> Were the reference standard results interpreted without knowledge of the results of the index test? 	Yes	"Both readers were blinded to the report and the RAPID software interpretation" (p. e46).
Risk of bias: Could the reference standard, its conduct, or its interpretation have introduced bias?	Low	'Yes' for all signalling questions.
B. Concerns regarding applicability		
Applicability: Is there concern that the target condition as defined by the reference standard does not match the review question?	Low	The target condition was LVO (i.e., ischemic stroke), and was likely to be correctly classified by the reference standard, which is directly relevant to the review question.
Domain 4: Flow and Timing		
A. Risk of Bias		
<ul style="list-style-type: none"> Was there an appropriate interval between index test(s) and reference standard? 	NA	Not applicable. The index test and the reference standard used the same CT images, and the timing of interpretation is not relevant.
<ul style="list-style-type: none"> Did all patients receive a reference standard? 	Yes	There were no indications that all patients did not receive a reference standard.
<ul style="list-style-type: none"> Did patients receive the same reference standard? 	Yes	All patients received the same reference standard.
<ul style="list-style-type: none"> Were all patients included in the analysis? 	No	13.7% (14 of 102) of patients were excluded from the analysis "due to technical difficulties" (p. e51). ⁵ It is not clear why these patients were excluded, and they may represent difficult to diagnose populations.
Risk of bias: Could the patient flow have introduced bias?	High	A large portion (13.7%) of the participants were excluded from the analysis for unknown reasons.

CT = computed tomography; CTA = computed tomography angiography; LVO = large vessel occlusion; NA = not applicable; QUADAS-2 = Quality Assessment of Diagnostic Accuracy Studies 2.

Table 11: Risk of Bias Assessment of Soun et al. (2023)¹ – QUADAS-2

Domain/question	Judgement	Comments
Domain 1: Patient Selection		
A. Risk of Bias		
<ul style="list-style-type: none"> Was a consecutive or random sample of patients enrolled? 	Yes	“This retrospective study included consecutive patients presenting with suspected acute ischemic stroke who had a CTA at a comprehensive stroke center” (p. 02). ¹
<ul style="list-style-type: none"> Was a case-control design avoided? 	Yes	Consecutive patients presenting with suspected acute ischemic stroke were included. Patient selection was independent of the results of the reference standard.
<ul style="list-style-type: none"> Did the study avoid inappropriate exclusions? 	Yes	The study excluded patients with technically inadequate CTA (e.g., poor contrast bolus, significant motion, or other artifacts that would preclude evaluation by both human and automated assessment). However, this is likely aligned with how the test would be used in practice.
Risk of bias: Could the selection of patients have introduced bias?	Low	‘Yes’ for all signalling questions.
B. Concerns regarding applicability		
Applicability: Is there concern that the included patients do not match the review question?	Low	Patients with clinical suspicion of acute ischemic stroke, which is directly relevant to the review question.
Domain 2: Index Test		
A. Risk of Bias		
<ul style="list-style-type: none"> Were the index test results interpreted without knowledge of the results of the reference standard? 	Yes	The study examined the diagnostic performance of Rapid LVO alone (which did not have access to the results of the reference standard)
<ul style="list-style-type: none"> If a threshold was used, was it pre-specified? 	Unclear	“The RAPID LVO algorithm which primarily relies on vessel density threshold assessment has been described previously” (p. 02). ¹ The threshold of relative vessel density for detecting LVO was not described.
Risk of bias: Could the conduct or interpretation of the index test have introduced bias?	Unclear	There is insufficient information to determine whether the threshold of relative vessel density for detecting LVO was pre-specified.
B. Concerns regarding applicability		
Applicability: Is there concern that the index test, its conduct, or interpretation differ from the review question?	High	The index test was Rapid LVO alone, which is different from our primary review question and how the tool is used in practice (i.e., Rapid LVO alongside clinician interpretation).
Domain 3: Reference Standard		

Domain/question	Judgement	Comments
A. Risk of Bias		
<ul style="list-style-type: none"> Is the reference standard likely to correctly classify the target condition? 	Yes	The reference standard was assessment of LVO on CTA from the radiologist's reports (with access to Rapid LVO results), which were verified by a board-certified neuroradiologist. For complex cases where the reference standard was not clearly delineated, 2 additional neuroradiologists determined the reference standard.
<ul style="list-style-type: none"> Were the reference standard results interpreted without knowledge of the results of the index test? 	No	The reference standard results were interpreted with knowledge of the analysis by Rapid LVO.
Risk of bias: Could the reference standard, its conduct, or its interpretation have introduced bias?	High	Knowledge of the index test results could have influenced the interpretation of the reference standard, which may bias estimates of agreement between the index test and the reference standard results.
B. Concerns regarding applicability		
Applicability: Is there concern that the target condition as defined by the reference standard does not match the review question?	Low	The target condition was LVO (i.e., ischemic stroke), and was likely to be correctly classified by the reference standard, which is directly relevant to the review question.
Domain 4: Flow and Timing		
A. Risk of Bias		
<ul style="list-style-type: none"> Was there an appropriate interval between index test(s) and reference standard? 	NA	Not applicable. The index test and the reference standard used the same CT images, and the timing of interpretation is not relevant.
<ul style="list-style-type: none"> Did all patients receive a reference standard? 	Yes	There were no indications that all patients did not receive a reference standard.
<ul style="list-style-type: none"> Did patients receive the same reference standard? 	Yes	The reference standard was consistent for all patients.
<ul style="list-style-type: none"> Were all patients included in the analysis? 	Unclear	The reporting related to the calculation of diagnostic performance metrics was limited. It was unclear if all 321 patients were included in the analysis.
Risk of bias: Could the patient flow have introduced bias?	Unclear	It is unclear if all patients were included in the analysis.

CT = computed tomography; CTA = computed tomography angiography; LVO = large vessel occlusion; NA = not applicable; QUADAS-2 = Quality Assessment of Diagnostic Accuracy Studies 2.

Table 12: Risk of Bias Assessment of Yedavalli et al. (2023)⁶ – QUADAS-2

Domain/question	Judgement	Comments
Domain 1: Patient Selection		
A. Risk of Bias		
<ul style="list-style-type: none"> Was a consecutive or random sample of patients enrolled? 	Unclear	<p>“Cases were obtained from consecutive emergency room (ER) scans obtained from Augusta University Medical Center and Riverside Regional Medical Center. Other hospitals that contributed cases included three community hospitals (Box Hill, Hospital de Clinicas, Olathe Medical Center) and two university centers (Kansas University Medical Center and, New York University). Two research studies that enrolled acute LVO patients, CRISP (9) and DEFUSE 3 (10) also contributed cases” (p. 02).⁶</p> <p>There is insufficient reporting of how the patient population was selected to determine if it was a consecutive or random sample.</p>
<ul style="list-style-type: none"> Was a case-control design avoided? 	Unclear	The methods for patient selection were unclear.
<ul style="list-style-type: none"> Did the study avoid inappropriate exclusions? 	Unclear	The eligibility criteria were not reported.
Risk of bias: Could the selection of patients have introduced bias?	Unclear	‘Unclear’ for all signalling questions.
B. Concerns regarding applicability		
Applicability: Is there concern that the included patients do not match the review question?	Low	Acutely presenting patients with suspected stroke, which is directly relevant to the review question.
Domain 2: Index Test		
A. Risk of Bias		
<ul style="list-style-type: none"> Were the index test results interpreted without knowledge of the results of the reference standard? 	Yes	The study examined the diagnostic performance of the Rapid NCCT Stroke platform alone (which did not have access to the results of the reference standard).
<ul style="list-style-type: none"> If a threshold was used, was it pre-specified? 	Yes	<p>“This AI software uses neural networks and automated segmentation techniques based on predefined thresholds for identification of ICH, HVS, and Alberta Stroke Program Early CT Score (ASPECTS)” (p. 03).⁶</p> <p>The authors indicated that the Rapid NCCT Stroke platform uses a predefined threshold for detecting the presence of a hyperdense vessel sign, so they likely used the threshold specified by the manufacturer of the test.</p>
Risk of bias: Could the conduct or interpretation of the index test have introduced bias?	Low	‘Yes’ for all signalling questions.

Domain/question	Judgement	Comments
B. Concerns regarding applicability		
Applicability: Is there concern that the index test, its conduct, or interpretation differ from the review question?	High	The index test was evaluation of NCCT by the Rapid NCCT Stroke platform (using the Rapid HVS to detect LVO) alone, which is different from our primary review question and how the tool is used in practice (i.e., Rapid NCCT Stroke platform alongside clinician interpretation).
Domain 3: Reference Standard		
A. Risk of Bias		
<ul style="list-style-type: none"> Is the reference standard likely to correctly classify the target condition? 	Yes	The reference standard diagnosis was based on a consensus of 2 of 3 neuroradiologists.
<ul style="list-style-type: none"> Were the reference standard results interpreted without knowledge of the results of the index test? 	Yes	“All readers performed interpretations blinded to the AI software results and clinical information. Readers then assessed for ICH, and if ICH was not present, they then assessed for suspected LVO. The reference truth for ICH was based on a consensus of two of three neuroradiologists evaluating the NCCT scan using the same parameters” (p. 03). ⁶
Risk of bias: Could the reference standard, its conduct, or its interpretation have introduced bias?	Low	‘Yes’ for all signalling questions.
B. Concerns regarding applicability		
Applicability: Is there concern that the target condition as defined by the reference standard does not match the review question?	Low	The target condition was LVO (i.e., ischemic stroke), and was likely to be correctly classified by the reference standard, which is directly relevant to the review question.
Domain 4: Flow and Timing		
A. Risk of Bias		
<ul style="list-style-type: none"> Was there an appropriate interval between index test(s) and reference standard? 	Yes	“Stand-alone performance was based on the reference LVO assessment which was determined by a consensus of two of three neuroradiologists based on a CTA performed concurrently with the NCCT” (p. 03). ⁶ Images used for the index test and the reference standard were conducted concurrently.
<ul style="list-style-type: none"> Did all patients receive a reference standard? 	Yes	There were no indications that all patients did not receive a reference standard.
<ul style="list-style-type: none"> Did patients receive the same reference standard? 	Yes	All patients received the same reference standard.
<ul style="list-style-type: none"> Were all patients included in the analysis? 	Unclear	“LVO: The software identified 73 true suspected LVOs (73/115, 63.5%) with 42 false negatives (42/115, 36.5%). It also correctly categorized 90 cases (90/115, 78.2%) where LVO was not present with five false positives (5/115, 4.3%). This resulted in a sensitivity of 63.5% (95% CI: 54.4–71.7%) and specificity of 95.1% (95% CI: 89.1–97.9%)” (p. 03). ⁶

Domain/question	Judgement	Comments
		There were inconsistencies in the reporting of the number of patients included in the analysis. The number of TP (n = 73), FP (n = 5), FN (n = 42), and TN (n = 90) sum to 210, but the total number of patients who had LVO or did not have LVO or ICH (the ICH-positive patients were considered in a separate analysis) was 218. The difference between these values was not explained.
Risk of bias: Could the patient flow have introduced bias?	Unclear	Unclear if all enrolled patients were included in the analysis; it appears as though data were missing for 8 (4%) patients, but no explanation is provided.

CT = computed tomography; CTA = computed tomography angiography; FN = false negative; FP = false positive; ICH = intracranial hemorrhage; LVO = large vessel occlusion; NA = not applicable; QUADAS-2 = Quality Assessment of Diagnostic Accuracy Studies 2; TN = true negative; TP = true positive.

DRAFT

Table 13: Risk of Bias Assessment of Eldaya et al. (2022)¹¹ – QUADAS-2

Domain/question	Judgement	Comments
Domain 1: Patient Selection		
A. Risk of Bias		
<ul style="list-style-type: none"> Was a consecutive or random sample of patients enrolled? 	Yes	“Three hundred eight consecutive adult patients presenting with acute neurological deficit suspicious for acute stroke and undergoing NCCT with RAPID ICH processing at a single large tertiary comprehensive stroke center with a large catchment area between May, 19, 2020, and October 16, 2020, were included (Fig. 1)” (p. 70). ¹¹
<ul style="list-style-type: none"> Was a case-control design avoided? 	Yes	Consecutive patients presenting with suspected acute stroke were included. Patient selection was independent of the results of the reference standard.
<ul style="list-style-type: none"> Did the study avoid inappropriate exclusions? 	Yes	“One patient was excluded from the study because of intravenous contrast administration a few hours before the NCCT confounding interpretation of a hyperdensity within the infarct as hemorrhage or contrast. The remaining 307 patients were included in the final analysis” (p. 771). ¹¹ Only 1/308 patients were excluded from the analysis, and rationale for exclusion was provided and reasonable.
Risk of bias: Could the selection of patients have introduced bias?	Low	‘Yes’ for all signalling questions.
B. Concerns regarding applicability		
Applicability: Is there concern that the included patients do not match the review question?	Low	Patients were those presenting with acute neurological deficit suspicious of acute stroke, which is directly relevant to the review question.
Domain 2: Index Test		
A. Risk of Bias		
<ul style="list-style-type: none"> Were the index test results interpreted without knowledge of the results of the reference standard? 	Yes	“Two neuroradiology fellows (M.Z. and E.M.) reviewed the patients’ electronic medical records to determine [...] presence and type of ICH reported in the neuroradiologist interpretation, and RAPID ICH result. For patients in whom RAPID ICH and neuroradiologist interpretation were concordant for the presence of ICH, the neuroradiologist interpretation was considered the reference standard. For patients in who RAPID ICH and neuroradiologist interpretation were discordant [...], a consensus panel of 3 board-certified neuroradiologists [...] was then used as the reference standard” (p. 771). ¹¹ The index test was conducted and interpreted before the reference standard.
<ul style="list-style-type: none"> If a threshold was used, was it pre-specified? 	Unclear	No threshold was reported.

Domain/question	Judgement	Comments
Risk of bias: Could the conduct or interpretation of the index test have introduced bias?	Unclear	'Yes' or 'Unclear' for all signalling questions.
B. Concerns regarding applicability		
Applicability: Is there concern that the index test, its conduct, or interpretation differ from the review question?	Low	The index test was RAPID ICH + neuroradiologist, which is directly applicable to the review question (and use of the tool in practice).
Domain 3: Reference Standard		
A. Risk of Bias		
<ul style="list-style-type: none"> Is the reference standard likely to correctly classify the target condition? 	Yes	When standalone Rapid ICH and neuroradiologist interpretation were concordant, it was considered the reference standard. In cases where there was disagreement between Rapid ICH and neuroradiologist interpretation, the reference standard was a consensus panel of 3 neuroradiologists (with 3, 6, and 24 years of experience).
<ul style="list-style-type: none"> Were the reference standard results interpreted without knowledge of the results of the index test? 	No	"The consensus panel was not blinded to the neuroradiologist interpretation nor the RAPID ICH result" (p. 771). ¹¹
Risk of bias: Could the reference standard, its conduct, or its interpretation have introduced bias?	High	In cases of concordance, the index test served as the reference standard, which could inflate the diagnostic accuracy of the index test. Additionally, in cases of discordance, the consensus panel of neuroradiologists was aware of the neuroradiologist interpretation and Rapid ICH result, which may bias the test accuracy estimates.
B. Concerns regarding applicability		
Applicability: Is there concern that the target condition as defined by the reference standard does not match the review question?	Low	The target condition was intracranial hemorrhage (i.e., hemorrhagic stroke), and was likely to be correctly classified by the reference standard, which is directly relevant to the review question
Domain 4: Flow and Timing		
A. Risk of Bias		
<ul style="list-style-type: none"> Was there an appropriate interval between index test(s) and reference standard? 	NA	Not applicable. The index test and the reference standard used the same CT images, and the timing of interpretation is not relevant.
<ul style="list-style-type: none"> Did all patients receive a reference standard? 	Yes	"For patients in whom RAPID ICH and neuroradiologist interpretation were concordant for the presence of ICH, the neuroradiologist interpretation was considered the reference standard. For patients in who RAPID ICH and neuroradiologist interpretation were discordant [...], a consensus panel of 3 board-certified neuroradiologists [...] was then used as the reference standard" (p. 771). ¹¹
<ul style="list-style-type: none"> Did patients receive the same reference standard? 	No	In some patients, the index test was considered the reference standard, while in others the reference standard was a consensus panel of 3 neuroradiologists (i.e., there was differential verification).



Domain/question	Judgement	Comments
<ul style="list-style-type: none">Were all patients included in the analysis?	Yes	The reporting was limited, but there were no indications that all 307 enrolled patients were not included in the analyses.
Risk of bias: Could the patient flow have introduced bias?	High	Different reference standards were used depending on the results of the index test, which could bias the accuracy estimates.

CT = computed tomography; CTA = computed tomography angiography; ICH = intracranial hemorrhage; LVO = large vessel occlusion; NA = not applicable; NCCT = non-contrast computed tomography; QUADAS-2 = Quality Assessment of Diagnostic Accuracy Studies 2.

DRAFT

Table 14: Risk of Bias Assessment of Mallon et al. (2022)⁷ – QUADAS-2

Domain/question	Judgement	Comments
Domain 1: Patient Selection		
A. Risk of Bias		
<ul style="list-style-type: none"> Was a consecutive or random sample of patients enrolled? 	Yes	"In this single-centre retrospective study, the cohort included all patients with either a suspected or confirmed anterior circulation LVO who underwent a CTP study at Imperial College NHS Healthcare Trust between 1 January 2016 and 31 December 2020" (p. 2). ⁷
<ul style="list-style-type: none"> Was a case-control design avoided? 	Yes	Patient selection was independent of the results of the reference standard.
<ul style="list-style-type: none"> Did the study avoid inappropriate exclusions? 	Yes	Only patients who did not have CTA imaging data available were excluded (4.4%; 4/90).
Risk of bias: Could the selection of patients have introduced bias?	Low	'Yes' for all signalling questions.
B. Concerns regarding applicability		
Applicability: Is there concern that the included patients do not match the review question?	Low	Patients were those who were being assessed for suspected or confirmed anterior circulation LVO, which is directly relevant to the review question.
Domain 2: Index Test		
A. Risk of Bias		
<ul style="list-style-type: none"> Were the index test results interpreted without knowledge of the results of the reference standard? 	Yes	The study examined the diagnostic performance of Rapid AI alone (which did not have access to the results of the reference standard).
<ul style="list-style-type: none"> If a threshold was used, was it pre-specified? 	Unclear	The threshold of relative vessel density for detecting LVO was not described.
Risk of bias: Could the conduct or interpretation of the index test have introduced bias?	Unclear	The threshold of relative vessel density for detecting LVO was not described.
B. Concerns regarding applicability		
Applicability: Is there concern that the index test, its conduct, or interpretation differ from the review question?	High	The index test was evaluation of CTA by Rapid AI alone, which is different from our primary review question and how the tool is used in practice (i.e., Rapid AI alongside clinician interpretation).
Domain 3: Reference Standard		
A. Risk of Bias		
<ul style="list-style-type: none"> Is the reference standard likely to correctly classify the target condition? 	Yes	The reference standard diagnosis was based assessment of CTA by a single neuroradiologist.

Domain/question	Judgement	Comments
<ul style="list-style-type: none"> Were the reference standard results interpreted without knowledge of the results of the index test? 	Unclear	<p>“ASPECTS was determined on NCCT and the presence of LVO on CTA by a neuroradiologist with 4 years’ experience. ASPECTS was determined as described previously. Images were reviewed with all available clinical and imaging data” (p.2).⁷</p> <p>It was not explicitly stated whether the reference standard assessments were conducted without knowledge of the index test results.</p>
Risk of bias: Could the reference standard, its conduct, or its interpretation have introduced bias?	Unclear	It is not clear whether the reference standard assessments were conducted without knowledge of the index test results.
B. Concerns regarding applicability		
Applicability: Is there concern that the target condition as defined by the reference standard does not match the review question?	Low	The target condition was LVO (i.e., ischemic stroke), and was likely to be correctly classified by the reference standard, which is directly relevant to the review question.
Domain 4: Flow and Timing		
A. Risk of Bias		
<ul style="list-style-type: none"> Was there an appropriate interval between index test(s) and reference standard? 	NA	Not applicable. The index test and the reference standard used the same CT images, and the timing of interpretation is not relevant.
<ul style="list-style-type: none"> Did all patients receive a reference standard? 	Yes	There were no indications that all patients did not receive a reference standard.
<ul style="list-style-type: none"> Did patients receive the same reference standard? 	Yes	All patients received the same reference standard.
<ul style="list-style-type: none"> Were all patients included in the analysis? 	No	1 of 90 participants was not included in the analysis because the algorithm failed to give an output.
Risk of bias: Could the patient flow have introduced bias?	Low	While not all patients were included in the analysis, the number of excluded patients is small (1.1% of the study population) and is unlikely to meaningfully bias the result.

ASPECTS = Alberta Stroke Program Early CT score; CT = computed tomography; CTA = computed tomography angiography; CTP = computed tomography perfusion; LVO = large vessel occlusion; NA = not applicable; NCCT = non-contrast computed tomography; QUADAS-2 = Quality Assessment of Diagnostic Accuracy Studies 2.

Table 15: Risk of Bias Assessment of Schlossman et al. (2022)⁸ – QUADAS-2

Domain/question	Judgement	Comments
Domain 1: Patient Selection		
A. Risk of Bias		
<ul style="list-style-type: none"> Was a consecutive or random sample of patients enrolled? 	Yes	<p>“This was a retrospective, single center study performed at University of California, Irvine, a comprehensive stroke center, using anonymized data from December 2020 to June 2021. Inclusion criteria was as follows: (1) suspected acute stroke patients who had CT angiography (CTA) performed, (2) imaging done within 24 h of symptom onset, and (3) RAPID LVO output included with CTA acquisition. Patients who had either (1) imaging acquired at outside facilities or (2) technically inadequate CTA (e.g., poor contrast bolus, significant motion, or other artifact that would preclude evaluation by both human and automated assessment) were excluded” (p. 02).⁸</p> <p>Based on the description of the study population, it appears to be a consecutively enrolled cohort of patients who met the eligibility criteria.</p>
<ul style="list-style-type: none"> Was a case-control design avoided? 	Yes	Patient selection was independent of the results of the reference standard.
<ul style="list-style-type: none"> Did the study avoid inappropriate exclusions? 	Yes	The study excluded patients with technically inadequate CTA (e.g., poor contrast bolus, significant motion, or other artifacts that would preclude evaluation by both human and automated assessment). However, this is likely aligned with how the test would be used in practice.
Risk of bias: Could the selection of patients have introduced bias?	Low	‘Yes’ for all signalling questions.
B. Concerns regarding applicability		
Applicability: Is there concern that the included patients do not match the review question?	Low	The study included patients with suspected acute stroke, which is directly relevant to the review question.
Domain 2: Index Test		
A. Risk of Bias		
<ul style="list-style-type: none"> Were the index test results interpreted without knowledge of the results of the reference standard? 	Yes	The study examined the diagnostic performance of Rapid LVO alone (which did not have access to the results of the reference standard).
<ul style="list-style-type: none"> If a threshold was used, was it pre-specified? 	Unclear	There is insufficient information to determine whether the threshold of relative vessel density for detecting LVO was pre-specified.
Risk of bias: Could the conduct or interpretation of the index test have introduced bias?	Unclear	It is unclear whether the threshold of relative vessel density for detecting LVO was pre-specified.
B. Concerns regarding applicability		

Domain/question	Judgement	Comments
Applicability: Is there concern that the index test, its conduct, or interpretation differ from the review question?	High	The index test was evaluation of CTA by Rapid LVO alone, which is different from our primary review question and how the tool is used in practice (i.e., Rapid LVO alongside clinician interpretation).
Domain 3: Reference Standard		
A. Risk of Bias		
<ul style="list-style-type: none"> Is the reference standard likely to correctly classify the target condition? 	Yes	The reference standard diagnosis was based on assessment of CTA by 2 neuroradiologists. Disagreements were adjudicated by a 3 rd neuroradiologist.
<ul style="list-style-type: none"> Were the reference standard results interpreted without knowledge of the results of the index test? 	Yes	<p>“Ground truth was based off interpretation of the raw data from the CTA by radiology reports and confirmed by two neuroradiologists” (p. 02).⁸</p> <p>Based on the above quote, it is likely that the reference standard was conducted using only the raw CTA data (i.e., without processing from Rapid LVO).</p>
Risk of bias: Could the reference standard, its conduct, or its interpretation have introduced bias?	Low	‘Yes’ for all signalling questions.
B. Concerns regarding applicability		
Applicability: Is there concern that the target condition as defined by the reference standard does not match the review question?	Low	The target condition was LVO (i.e., ischemic stroke), and was likely to be correctly classified by the reference standard, which is directly relevant to the review question.
Domain 4: Flow and Timing		
A. Risk of Bias		
<ul style="list-style-type: none"> Was there an appropriate interval between index test(s) and reference standard? 	NA	Not applicable. The index test and the reference standard used the same CT images, and the timing of interpretation is not relevant.
<ul style="list-style-type: none"> Did all patients receive a reference standard? 	Yes	There were no indications that all patients did not receive a reference standard.
<ul style="list-style-type: none"> Did patients receive the same reference standard? 	Yes	All patients received the same reference standard.
<ul style="list-style-type: none"> Were all patients included in the analysis? 	Yes	All 253 patients were included in the Rapid LVO confusion matrix and the calculation of diagnostic parameters.
Risk of bias: Could the patient flow have introduced bias?	Low	‘Yes’ for all signalling questions.

CT = computed tomography; CTA = computed tomography angiography; LVO = large vessel occlusion; NA = not applicable; QUADAS-2 = Quality Assessment of Diagnostic Accuracy Studies 2.

Table 16: Risk of Bias Assessment of Adhya et al. (2021)² – QUADAS-2

Domain/ signalling question	Judgement	Comments
Domain 1: Patient Selection		
A. Risk of Bias		
<ul style="list-style-type: none"> Was a consecutive or random sample of patients enrolled? 	Yes	<p>“All patients who received CTA for the evaluation of AIS or neurological deficit from November 2019–November 2020 that included RAPID-CTA with relative vessel density of 60% or less were included in the study” (p. 4).²</p> <p>Based on the description of the study population, it appears to be a consecutively enrolled cohort of patients who met the eligibility criteria.</p>
<ul style="list-style-type: none"> Was a case-control design avoided? 	Yes	Patient selection was independent of the results of the reference standard.
<ul style="list-style-type: none"> Did the study avoid inappropriate exclusions? 	No	Patients with a relative vessel density of 60% or more were excluded, which makes for a selected population that is not reflective of clinical practice. These could represent patients who are negative for LVO or who have LVO but are difficult to diagnose populations.
Risk of bias: Could the selection of patients have introduced bias?	High	The study applied inappropriate exclusion criteria and selected for a population that is not reflective of clinical practice.
B. Concerns regarding applicability		
Applicability: Is there concern that the included patients do not match the review question?	Low	Patients were those who underwent CTA for the evaluation of acute ischemic stroke or neurological deficit, which is directly relevant to the review question.
Domain 2: Index Test		
A. Risk of Bias		
<ul style="list-style-type: none"> Were the index test results interpreted without knowledge of the results of the reference standard? 	Yes	The study examined the diagnostic performance of Rapid CTA alone (which did not have access to the results of the reference standard).
<ul style="list-style-type: none"> If a threshold was used, was it pre-specified? 	Yes	Two thresholds were tested (i.e., < 45% relative vessel density and < 60% relative vessel density) and were likely pre-specified.
Risk of bias: Could the conduct or interpretation of the index test have introduced bias?	Low	‘Yes’ for all signalling questions.
B. Concerns regarding applicability		
Applicability: Is there concern that the index test, its conduct, or interpretation differ from the review question?	High	The index test was evaluation of CTA by Rapid CTA alone, which is different from our primary review question and how the tool is used in practice (i.e., Rapid CTA alongside clinician interpretation).
Domain 3: Reference Standard		

Domain/ signalling question	Judgement	Comments
A. Risk of Bias		
<ul style="list-style-type: none"> Is the reference standard likely to correctly classify the target condition? 	Yes	The reference standard diagnosis was based on assessment of CTA by 2 neuroradiologists.
<ul style="list-style-type: none"> Were the reference standard results interpreted without knowledge of the results of the index test? 	Unclear	It was not explicitly stated whether the reference standard assessments were conducted without knowledge of the index test results.
Risk of bias: Could the reference standard, its conduct, or its interpretation have introduced bias?	Unclear	It is not clear whether the reference standard assessments were conducted without knowledge of the index test results.
B. Concerns regarding applicability		
Applicability: Is there concern that the target condition as defined by the reference standard does not match the review question?	Low	The target condition was LVO (i.e., ischemic stroke), and was likely to be correctly classified by the reference standard, which is directly relevant to the review question.
Domain 4: Flow and Timing		
A. Risk of Bias		
<ul style="list-style-type: none"> Was there an appropriate interval between index test(s) and reference standard? 	NA	Not applicable. The index test and the reference standard used the same CT images, and the timing of interpretation is not relevant.
<ul style="list-style-type: none"> Did all patients receive a reference standard? 	Yes	There were no indications that all patients did not receive a reference standard.
<ul style="list-style-type: none"> Did patients receive the same reference standard? 	Yes	All patients received the same reference standard.
<ul style="list-style-type: none"> Were all patients included in the analysis? 	Yes	There were no indications to suggest that all patients were not included in the analysis.
Risk of bias: Could the patient flow have introduced bias?	Low	'Yes' or 'NA' for all signalling questions.

CT = computed tomography; CTA = computed tomography angiography; LVO = large vessel occlusion; NA = not applicable; QUADAS-2 = Quality Assessment of Diagnostic Accuracy Studies 2.



Table 17: Risk of Bias Assessment of Dehkharghani et al. (2021)⁹ – QUADAS-2

Domain and questions	Judgement	Comments
Domain 1: Patient Selection		
A. Risk of Bias		
<ul style="list-style-type: none"> Was a consecutive or random sample of patients enrolled? 	No	Patients were enrolled from recent cerebrovascular trials and institutional registries from 11 worldwide sites were included and selected for inclusion using LVO status, location, CT vendor, and baseline demographics (i.e., a non-random and non-consecutive sample).
<ul style="list-style-type: none"> Was a case-control design avoided? 	No	The study population was enriched with patients who had known LVO status to achieve balance between LVO-positive and LVO-negative patients (i.e., it is a case-control selected cross-sectional study).
<ul style="list-style-type: none"> Did the study avoid inappropriate exclusions? 	Yes	The study excluded patients who did not have "...technically adequate thin section (≤ 2 mm section thickness) contiguous cerebrovascular CTA source axial images free of artifacts that would degrade interpretation by human readers (e.g., those related to severe metallic streak or beam hardening)" (p. 666). ⁹ However, this is likely aligned with how the test would be used in practice.
Risk of bias: Could the selection of patients have introduced bias?	High	The study included a non-consecutive and non-random patient population and provided limited reporting on the methods used to select patients for inclusion.
B. Concerns regarding applicability		
Applicability: Is there concern that the included patients do not match the review question?	Low	The study included patients with suspected acute ischemic stroke who underwent CTA imaging, which is directly relevant to the review question.
Domain 2: Index Test		
A. Risk of Bias		
<ul style="list-style-type: none"> Were the index test results interpreted without knowledge of the results of the reference standard? 	Yes	The study examined the diagnostic performance of Rapid LVO alone (which did not have access to the results of the reference standard).
<ul style="list-style-type: none"> If a threshold was used, was it pre-specified? 	Unclear	<p>"A custom vessel tracking algorithm (RapidLVO, version 1.0; iSchemaView) was used to inform the course, caliber, opacity, and continuity of the filtered vasculature, and vascular opacification was quantified with density thresholding. The thresholding operation represents a tunable parameter described by a vessel density ratio. By default, a vascular segment failing to reach the terminus of a predefined region of interest is classified as a vessel density ratio of 0.0. With a potential vessel density ratio ranging from 0.00 to 1.00, a score less than 0.6 was classified as positive for the presence of LVO" (p. 666).⁹</p> <p>It was not stated whether the vessel density ratio threshold for the primary analyses was pre-defined or selected post-hoc.</p>
Risk of bias: Could the conduct or interpretation of the index test have introduced bias?	Unclear	It is not clear whether the vessel density ratio threshold for the primary analyses was pre-defined or selected post-hoc.

Domain and questions	Judgement	Comments
B. Concerns regarding applicability		
Applicability: Is there concern that the index test, its conduct, or interpretation differ from the review question?	High	The index test was evaluation of CTA by Rapid LVO alone, which is different from our primary review question and how the tool is used in practice (i.e., Rapid LVO alongside clinician interpretation).
Domain 3: Reference Standard		
A. Risk of Bias		
<ul style="list-style-type: none"> Is the reference standard likely to correctly classify the target condition? 	Yes	The reference standard diagnosis was based on assessment of CTA by consensus from up to 3 neuroradiologists.
<ul style="list-style-type: none"> Were the reference standard results interpreted without knowledge of the results of the index test? 	Yes	“Readers 1 and 2 independently scored all examinations for LVO and, when present, the side of the LVO, before receiving the automated output. Once submitted, reader scores could not be modified” (p. 666). ⁹
Risk of bias: Could the reference standard, its conduct, or its interpretation have introduced bias?	Low	‘Yes’ for all signalling questions.
B. Concerns regarding applicability		
Applicability: Is there concern that the target condition as defined by the reference standard does not match the review question?	Low	The target condition was LVO (i.e., ischemic stroke), and was likely to be correctly classified by the reference standard, which is directly relevant to the review question.
Domain 4: Flow and Timing		
A. Risk of Bias		
<ul style="list-style-type: none"> Was there an appropriate interval between index test(s) and reference standard? 	NA	Not applicable. The index test and the reference standard used the same CT images, and the timing of interpretation is not relevant.
<ul style="list-style-type: none"> Did all patients receive a reference standard? 	Yes	There were no indications that all patients did not receive a reference standard.
<ul style="list-style-type: none"> Did patients receive the same reference standard? 	Yes	All patients received the same reference standard.
<ul style="list-style-type: none"> Were all patients included in the analysis? 	Yes	All 217 patients were included in the Rapid LVO confusion matrix and the calculation of diagnostic parameters.
Risk of bias: Could the patient flow have introduced bias?	Low	‘Yes’ or ‘NA’ for all signalling questions.

CT = computed tomography; CTA = computed tomography angiography; LVO = large vessel occlusion; NA = not applicable; QUADAS-2 = Quality Assessment of Diagnostic Accuracy Studies 2.

Table 18: Risk of Bias Assessment of Amukotuwa et al. (2019)¹⁰ – QUADAS-2

Domain/ signalling question	Judgement	Comments
Domain 1: Patient Selection		
A. Risk of Bias		
<ul style="list-style-type: none"> Was a consecutive or random sample of patients enrolled? 	Yes	“Consecutive patients who presented to our institution between January 1, 2017 and December 31, 2018 underwent multimodal brain CT for a suspected acute ischemic stroke and met the following inclusion criteria were retrospectively identified using our Picture Archiving and Communication System and electronic medical records” (p. 2791). ¹⁰
<ul style="list-style-type: none"> Was a case-control design avoided? 	Yes	Consecutive patients with suspected acute ischemic stroke were included. Patient selection was independent of the results of the reference standard.
<ul style="list-style-type: none"> Did the study avoid inappropriate exclusions? 	Yes	“Exclusion criteria were (1) technically inadequate CTA (poor contrast bolus or substantial motion of metal artifact that precluded accurate assessment of the intracranial arteries to the level of the distal M2 segments of the middle cerebral arteries by an experienced neurologist) and (2) thin slice CTA images unavailable” (p. 2791). ¹⁰ However, this is likely aligned with how the test would be used in practice.
Risk of bias: Could the selection of patients have introduced bias?	Low	‘Yes’ for all signalling questions.
B. Concerns regarding applicability		
Applicability: Is there concern that the included patients do not match the review question?	Low	The study included patients with suspected acute ischemic stroke who underwent multimodal brain CT, which is directly relevant to the review question.
Domain 2: Index Test		
A. Risk of Bias		
<ul style="list-style-type: none"> Were the index test results interpreted without knowledge of the results of the reference standard? 	Yes	The study examined the diagnostic performance of Rapid CTA alone (which did not have access to the results of the reference standard).
<ul style="list-style-type: none"> If a threshold was used, was it pre-specified? 	Yes	“A vessel density threshold of < 75% (inclusive of the 60%–75%, 45%–59%, and < 45% thresholds) was used in this study for LVO detection, as this was recommended by the software developers based on their prerelease testing” (p. 2792). ¹⁰ A rationale was provided for selecting the vessel density threshold. It is likely that this was determined before conducting the analysis.
Risk of bias: Could the conduct or interpretation of the index test have introduced bias?	Low	‘Yes’ for all signalling questions.
B. Concerns regarding applicability		

Domain/ signalling question	Judgement	Comments
Applicability: Is there concern that the index test, its conduct, or interpretation differ from the review question?	High	The index test was evaluation of CTA by Rapid CTA alone, which is different from our primary review question and how the tool is used in practice (i.e., Rapid CTA alongside clinician interpretation).
Domain 3: Reference Standard		
A. Risk of Bias		
<ul style="list-style-type: none"> Is the reference standard likely to correctly classify the target condition? 	Yes	The reference standard diagnosis was based on consensus assessment of LVO on unenhanced CT, CTP, and CTA by 2 diagnostic neuroradiologists. A 3 rd interventional neuroradiologist verified decisions.
<ul style="list-style-type: none"> Were the reference standard results interpreted without knowledge of the results of the index test? 	Yes	<p>“The multimodal computed tomographies were assessed by 2 neuroradiologists in consensus for the presence of an intracranial anterior circulation LVO or M2-segment middle cerebral artery occlusion (the reference standard). The patients’ computed tomography angiographies were then processed using an automated LVO-detection algorithm (RAPID CTA)” (p. 2790).¹⁰</p> <p>Based on the above quote, it is likely that the reference standard was conducted before the index test (and therefore the results of the index test could not have influenced the reference standard).</p>
Risk of bias: Could the reference standard, its conduct, or its interpretation have introduced bias?	Low	‘Yes’ for all signalling questions.
B. Concerns regarding applicability		
Applicability: Is there concern that the target condition as defined by the reference standard does not match the review question?	Low	The target condition was LVO (i.e., ischemic stroke), and was likely to be correctly classified by the reference standard, which is directly relevant to the review question.
Domain 4: Flow and Timing		
A. Risk of Bias		
<ul style="list-style-type: none"> Was there an appropriate interval between index test(s) and reference standard? 	NA	Not applicable. The index test and the reference standard used the same CT images, and the timing of interpretation is not relevant.
<ul style="list-style-type: none"> Did all patients receive a reference standard? 	Yes	There were no indications that all patients did not receive a reference standard.
<ul style="list-style-type: none"> Did patients receive the same reference standard? 	Yes	All patients received the same reference standard.
<ul style="list-style-type: none"> Were all patients included in the analysis? 	Yes	All 477 patients who met eligibility criteria were included in analysis.
Risk of bias: Could the patient flow have introduced bias?	Low	Yes’ or ‘NA’ for all signalling questions.

CT = computed tomography; CTA = computed tomography angiography; LVO = large vessel occlusion; NA = not applicable; QUADAS-2 = Quality Assessment of Diagnostic Accuracy Studies 2.

Main Study Findings

Table 19: Study Results, by Outcome — Time to Intervention

Study citation	Study design	Intervention and comparator	Outcome	Outcome result		P value
				Pre-RapidAI	Post-RapidAI	
Soun et al. (2023) ¹	Retrospective non-concurrent cohort	I: Clinician interpretation of CTA imaging with Rapid LVO (i.e., post-RapidAI group) C: Clinician interpretation of CTA imaging without Rapid LVO (i.e., pre-RapidAI group)	Radiology report turnaround time (minutes), ^a mean (SD)	30.58 (29.85) (n ≤ 439) ^b	22 (35.07) (n ≤ 321) ^b	0.0005 ^{c,d}
			Time from door to image (minutes), median (IQR)	11 (8 to 20) (n ≤ 62) ^b	13 (7 to 20) (n ≤ 43) ^b	0.75 ^e
			Time from door to intubation (minutes), median (IQR)	64.5 (46 to 73) (n ≤ 62) ^b	69.5 (58 to 86) (n ≤ 43) ^b	0.15 ^e
			Time from door to needle (i.e., tPA therapy) (minutes), median (IQR)	37 (25.5 to 44) (n ≤ 62) ^b	42 (30 to 53) (n ≤ 43) ^b	0.38 ^e
			Time from door to groin puncture (i.e., thrombectomy) (minutes), median (IQR)	97 (80 to 107) (n ≤ 62)	101 (90 to 113) (n ≤ 43) ^b	0.32 ^e
			Time from door to revascularization (minutes), median (IQR)	155 (123 to 197) (n ≤ 62) ^b	158 (131 to 191.5) (n ≤ 43) ^b	0.72 ^e
Adhya et al. (2021) ²	Retrospective non-concurrent cohort	I: Clinician interpretation of CTA imaging with Rapid CTA (i.e., post-RapidAI group) C: Clinician interpretation of CTA imaging without Rapid CTA (i.e., pre-RapidAI group)	Time from CTA to groin puncture (i.e., thrombectomy) (minutes), mean (SD)	92 (NR) (n = 74)	68 (NR) (n = 72)	< 0.05 ^{c,d}

C = comparator; CTA = computed tomography angiography; I = intervention; IQR = interquartile range; LVO = large vessel occlusion; NR = not reported; SD = standard deviation; tPA = tissue plasminogen activator.

^a Defined as the time from when the CTA images are available for the radiologist to the earlier time of either the report being available or read-back verification was provided for the clinicians.

^b The sample size for the analysis was not explicitly reported; as such, the amount of missing data is unknown.

^c Statistically significant.

^d Statistical test not reported (Student's t-test or Mann-Whitney U test).

^e Wilcoxon rank sum test.

Table 20: Study Results, by Outcome — Functional Status

Study citation	Study design	Intervention and comparator	Outcome	Outcome result		P value
				Pre-RapidAI	Post-RapidAI	
Soun et al. (2023) ¹	Retrospective non-concurrent cohort	I: Clinician interpretation of CTA imaging with Rapid LVO (i.e., post-RapidAI group) C: Clinician interpretation of CTA imaging without Rapid LVO (i.e., pre-RapidAI group)	36-hour post-treatment NIHSS score, median (IQR) ^a	9.5 (5 to 18) (n = NR) ^b	11 (2 to 20) (n = NR) ^b	0.71 ^c
			NIHSS score at discharge, median (IQR) ^a	4.5 (1 to 11) (n = NR) ^b	8 (1.5 to 20) (n = NR) ^b	0.099 ^c
			Change in NIHSS score from admission to discharge, median (IQR) ^a	-7 (-2 to -13) (n = NR) ^b	-3 (0 to -7) (n = NR) ^b	0.03 ^{c,d}
			Proportion of patients with mRS score ≥ 5 at discharge, n/N ^{e,f}	11/62 (17.7%)	10/43 (23.3%)	0.62 ^c
Adhya et al. (2021) ²	Retrospective non-concurrent cohort	I: Clinician interpretation of CTA imaging with Rapid CTA (i.e., post-RapidAI group) C: Clinician interpretation of CTA imaging without Rapid CTA (i.e., pre-RapidAI)	90-day mRS score, mean (SD) ^e	4.47 (NR) (n = 74)	3.90 (NR) (n = 67)	0.07 ^g
			Proportion of patients with 90-day mRS score ≤ 2 , n/N ^{e,h}	17/74 (23.0%)	23/67 (34.3%)	0.15 ^g

C = comparator; CTA = computed tomography angiography; I = intervention; IQR = interquartile range; LVO = large vessel occlusion; mRS = modified Rankin Scale; NIHSS = National Institutes of Health Stroke Scale; NR = not reported; SD = standard deviation.

^a The National Institutes of Health Stroke Scale is a 15-item neurological examination stroke scale used for evaluating stroke-related neurological deficit. Total scores range from 0 to 42, with higher scores indicating more severe neurological deficit.¹²

^b The sample size for the analysis was not explicitly reported; as such, the amount of missing data is unknown. The analyses for Thrombolysis in Cerebral Infarction scores and mRS scores included 62 and 46 participants in the pre-RapidAI group and 46 and 34 participants in the post-RapidAI group, respectively, but it is unclear if these samples sizes are applicable to other clinical outcomes.

^c Wilcoxon rank sum test. After adjusting for the effects of high cholesterol, heart disease, atrial fibrillation, therapies received, and NIHSS on admission via multivariate regression, the P value for the between-group difference in NIHSS score at discharge was < 0.01 . The between-group difference for 36-hour post-treatment NIHSS score was not statistically significant when adjusted for the same variables (P value not reported).

^d Statistically significant.

^e The modified Rankin Scale is a clinician-reported tool for measuring the degree of disability and dependence in daily activities in people who have experienced stroke. Scores range from 0 (no symptoms at all) to 6 (death). A higher score indicates greater disability.¹³

^f Considered 'significant morbidity/mortality'.

^g Statistical test not reported (Student's t-test or Mann-Whitney U test).

^h Considered 'functionally independent'.



Table 21: Study Results, by Outcome — Response to Therapy

Study citation	Study design	Intervention and comparator	Outcome	Outcome result		P value
				Pre-RapidAI	Post-RapidAI	
Soun et al. (2023) ¹	Retrospective non-concurrent cohort	I: Clinician interpretation of CTA imaging with Rapid LVO (i.e., post-RapidAI group) C: Clinician interpretation of CTA imaging without Rapid LVO (i.e., pre-RapidAI group)	Proportion of patients with TICl score of 0, n/N ^a	2/46 (4.3%)	3/34 (8.8%)	0.51 ^b
			Proportion of patients with TICl score of 1, n/N ^a	1/46 (2.2%)	0/34 (0%)	
			Proportion of patients with TICl score of 2A, n/N ^a	4/46 (8.7%)	4/34 (11.8%)	
			Proportion of patients with TICl score of 2B/C, n/N ^a	18/46 (39.1%)	17/34 (50.0%)	
			Proportion of patients with TICl score of 3, n/N ^a	21/46 (45.7%)	10/34 (29.4%)	

C = comparator; CTA = computed tomography angiography; I = intervention; IQR = interquartile range; LVO = large vessel occlusion; NR = not reported; TICl = Thrombolysis in Cerebral Infarction.

^a The Thrombolysis in Cerebral Infarction (TICl) scale is a grading system used to evaluate the degree of perfusion obtained following recanalization of an arterial occlusion. The TICl scale ranges from 0 (no reperfusion) to 3 (complete reperfusion).¹⁴

^b Chi-squared test.

Table 22: Study Results, by Outcome — Diagnostic Accuracy for the Detection of M1 MCA and ICA LVO

Study Citation	Index Test and Reference Standard	Type of LVO and Subgroup (if applicable)	TP	FP	FN	TN	Sensitivity (95% CI)	Specificity (95% CI)	PPV (95% CI)	NPV (95% CI)	AUC (95% CI)
Chan et al. (2023) ⁵ (N = 88)	IT: Rapid CTA alone RS: Consensus of 2 neuroradiologists	M1 MCA and terminal ICA LVO	12	11	1	64	92% (64 to 100) ^a	85% (75 to 92) ^a	52% (31 to 73) ^a	98% (92 to 100) ^a	NR
Soun et al. (2023) ¹ (N = 321)	IT: Rapid LVO alone RS: Single radiologist report, verified by up to 3 additional neuroradiologists	M1 MCA and intracranial ICA LVO	NR	NR	NR	NR	96% (NR)	85% (NR)	53% (NR)	99% (NR)	NR
Yedavalli et al. (2023) ⁶ (N = 244)	IT: Rapid NCCT Stroke platform alone ^b RS: Consensus of 2 of 3 neuroradiologists	M1 MCA and distal intracranial ICA LVO	73	5	42	90	63% (54 to 72)	95% (88 to 98) ^c	94% (86 to 98) ^{a,d}	68% (60 to 76) ^{a,d}	NR
Schlossman et al. (2022) ⁸ (N = 253)	IT: Rapid LVO alone RS: Consensus of 2 neuroradiologists	M1 MCA and intracranial ICA LVO	26	32	3	192	90% (73 to 98) ^a	86% (80 to 90) ^a	45% (32 to 58) ^a	98% (96 to 100) ^a	NR
Dehkharghani et al. (2021) ⁹ (N = 217)	Index test: Rapid LVO alone Reference standard: Consensus of up to 3 neuroradiologists	M1 MCA and intracranial ICA LVO	105	2	4	106	96% (91 to 99)	98% (94 to 100)	NA ^e	NA ^e	NR
		M1 MCA and intracranial ICA LVO Subgroup: female (n = 100)	52	0	2	46	96% (87 to 100)	100% (92 to 100)	NA ^e	NA ^e	NR
		M1 MCA and intracranial ICA LVO Subgroup: male (n = 116)	52	2	2	60	96% (87 to 100)	97% (89 to 100)	NA ^e	NA ^e	NR
		M1 MCA and intracranial ICA LVO Subgroup: 20 to 39 years of age (n = 17)	7	0	0	10	100% (59 to 100)	100% (69 to 100)	NA ^e	NA ^e	NR

Study Citation	Index Test and Reference Standard	Type of LVO and Subgroup (if applicable)	TP	FP	FN	TN	Sensitivity (95% CI)	Specificity (95% CI)	PPV (95% CI)	NPV (95% CI)	AUC (95% CI)
		M1 MCA and intracranial ICA LVO Subgroup: 40 to 59 years of age (n = 68)	29	1	0	38	100% (88 to 100)	97% (87 to 100)	NA ^e	NA ^e	NR
		M1 MCA and intracranial ICA LVO Subgroup: ≥ 60 years of age (n = 131)	69	1	4	57	95% (87 to 98)	98% (91 to 100)	NA ^e	NA ^e	NR
Amukotuwa et al. (2019) ¹⁰ (N = 477)	IT: Rapid CTA alone RS: Consensus of 2 neuroradiologists, verified by a 3 rd neuroradiologist	M1 MCA and intracranial ICA LVO	73	NR	5	NR	94% (86 to 98)	76% (72 to 80)	43% (39 to 48)	98% (96 to 99)	0.85 (0.81 to 0.88)

AUC = area under the receiver operating characteristic curve; CTA = computed tomography angiography; FN = false negatives; FP = false positives; ICA = internal carotid artery; IT = index test; LVO = large vessel occlusion; MCA = middle cerebral artery; NCCT = non-contrast computed tomography; NPV = negative predictive value; NR = not reported; PPV = positive predictive value; TN = true negatives; TP = true positives; RS = reference standard.

^a Not reported in the publication. We calculated the value with Clopper-Pearson exact 95% confidence intervals from the available data via the EpiR package in R.¹⁵

^b Unlike other index tests included in this table, the Rapid NCCT Stroke platform detects LVO using NCCT images (rather than CTA images).

^c Reported as 95% (89 to 98) in the publication, but was calculated as 95% (88 to 98) via the EpiR package in R.¹⁵

^d Patient selection methods were unclear.

^e PPV and NPV values were not calculated for Dehkharghani et al. (2019) as it used a case-control selected cross-sectional design that artificially created a sample of equally divided LVO-positive and LVO-negative patients.



Table 23: Study Results, by Outcome — Diagnostic Accuracy for the Detection of M1 and M2 MCA and ICA LVO

Study Citation	Index Test and Reference Standard	Type of LVO and Subgroup (if applicable)	TP	FP	FN	TN	Sensitivity (95% CI)	Specificity (95% CI)	PPV (95% CI)	NPV (95% CI)	AUC (95% CI)
Mallon et al. (2022) ⁷ (N = 84)	IT: RapidAI alone RS: A single neuroradiologist	M1 and M2 MCA and terminal ICA LVO	45	8	16	15	74% (61 to 84) ^a	65% (43 to 84) ^a	85% (72 to 93) ^a	48% (30 to 67) ^a	NR
Amukotuwa et al. (2019) ¹⁰ (N = 477)	IT: Rapid CTA alone RS: Consensus of 2 neuroradiologists, verified by a 3 rd neuroradiologist	M1 and M2 MCA and intracranial ICA LVO	97	71	9	300	92% (85 to 96)	81% (77 to 85)	58% (52 to 63)	97% (95 to 98)	0.86 (0.83 to 0.90)

AUC = area under the receiver operating characteristic curve; FN = false negatives; FP = false positives; ICA = internal carotid artery; IT = index test; LVO = large vessel occlusion; MCA = middle cerebral artery; NPV = negative predictive value; NR = not reported; PPV = positive predictive value; TN = true negatives; TP = true positives; RS = reference standard.

^a Not reported in the publication. We calculated the value with Clopper-Pearson exact 95% confidence intervals from the available data via the EpiR package in R.¹⁵



Table 24: Study Results, by Outcome — Diagnostic Accuracy for the Detection of M1 MCA LVO

Study Citation	Index Test and Reference Standard	Type of LVO and Subgroup (if applicable)	TP	FP	FN	TN	Sensitivity (95% CI)	Specificity (95% CI)	PPV (95% CI)	NPV (95% CI)	AUC (95% CI)
Mallon et al. (2022) ⁷ (N = 84)	IT: RapidAI alone RS: A single neuroradiologist	M1 MCA LVO (n = 73)	33	8	4	27	89% (75 to 97) ^a	77% (60 to 90) ^a	80% (65 to 91) ^a	87% (70 to 96) ^a	NR
Schlossman et al. (2022) ⁸ (N = 253)	IT: Rapid LVO alone RS: Consensus of 2 neuroradiologists	M1 MCA LVO (n = 247)	21	32	2	192	91% (72 to 99) ^a	86% (80 to 90) ^a	40% (26 to 54) ^a	99% (96 to 100) ^a	NR

AUC = area under the receiver operating characteristic curve; FN = false negatives; FP = false positives; IT = index test; LVO = large vessel occlusion; MCA = middle cerebral artery; NPV = negative predictive value; NR = not reported; PPV = positive predictive value; TN = true negatives; TP = true positives; RS = reference standard.

^a Not reported in the publication. We calculated the value with Clopper-Pearson exact 95% confidence intervals from the available data via the EpiR package in R.¹⁵

DRAFT



Table 25: Study Results, by Outcome — Diagnostic Accuracy for the Detection of M2 MCA LVO

Study Citation	Index Test and Reference Standard	Type of LVO and Subgroup (if applicable)	TP	FP	FN	TN	Sensitivity (95% CI)	Specificity (95% CI)	PPV (95% CI)	NPV (95% CI)	AUC (95% CI)
Schlossman et al. (2022) ⁸ (N = NR)	IT: Rapid LVO alone RS: Consensus of 2 neuroradiologists	M2 MCA LVO	8	NR	2	NR	80% (NR)	NR	NR	NR	NR
Amukotuwa et al. (2019) ¹⁰ (N = 477)	IT: Rapid CTA alone RS: Consensus of 2 neuroradiologists, verified by a 3 rd neuroradiologist	M2 MCA LVO	24	NR	4	NR	86% (67 to 96)	68% (63 to 72)	14% (12 to 17)	99% (97 to 100)	0.77 (0.70 to 0.84)

AUC = area under the receiver operating characteristic curve; FN = false negatives; FP = false positives; IT = index test; LVO = large vessel occlusion; MCA = middle cerebral artery; NPV = negative predictive value; NR = not reported; PPV = positive predictive value; TN = true negatives; TP = true positives; RS = reference standard.

Table 26: Study Results, by Outcome — Diagnostic Accuracy for the Detection of Other LVO

Study Citation	Index Test and Reference Standard	Type of LVO and Subgroup (if applicable)	TP	FP	FN	TN	Sensitivity (95% CI)	Specificity (95% CI)	PPV (95% CI)	NPV (95% CI)	AUC (95% CI)
Delora et al. (2024) ³ (N = 360)	IT: Rapid LVO alone RS: Interpretation by a single neuroradiologist	LVO ^a	41	48	6	265	87% (74 to 95) ^b	85% (80 to 88) ^b	46% (35 to 57) ^b	98% (95 to 99) ^{b,c}	NR
Slater et al. (2024) ⁴ (N = 500)	IT: Rapid LVO alone RS: Consensus of 3 or 4 neuroradiologists	LVO of the intracranial ICA, M1 or M2 MCA segments, basilar artery, or intracranial vertebral artery	NR	NR	NR	NR	62% (48 to 75)	93% (90 to 95)	NR	NR	NR
Schlossman et al. (2022) ⁸ (N = 253)	IT: Rapid LVO alone RS: Consensus of 2 neuroradiologists	Intracranial ICA LVO (n = 235)	9	32	2	192	82% (48 to 98) ^b	86% (80 to 90) ^b	22% (11 to 38) ^b	99% (96 to 100) ^b	NR
Adhya et al. (2021) ² (N = 310)	IT: Rapid CTA alone at < 45% relative vessel density threshold RS: Consensus of 2 neuroradiologists	LVO ^a	129	43	32	106	80% (73 to 86) ^b	71% (63 to 78) ^b	75% (68 to 81) ^b	77% (69 to 84) ^b	NR
	IT: Rapid CTA alone at ≤ 60% relative vessel density threshold RS: Consensus of 2 neuroradiologists	LVO ^a	161	149	0	0	NE ^d	NE ^d	NE	NE	NR

AUC = area under the receiver operating characteristic curve; FN = false negatives; FP = false positives; ICA = internal carotid artery; IT = index test; LVO = large vessel occlusion; MCA = middle cerebral artery; NE = not estimable; NPV = negative predictive value; NR = not reported; PPV = positive predictive value; TN = true negatives; TP = true positives; RS = reference standard.

^a Unclear which types of LVO were considered eligible. In Delora et al. (2024),³ the study population included patients with occlusions of the ICA, M1 MCA segment, and M2 MCA segment. The study population from Adhya et al. (2021) included patients with occlusions of the ICA, carotid terminus, M1 MCA segment, and M2 MCA segment.

^b Not reported in the publication. We calculated the value with Clopper-Pearson exact 95% confidence intervals from the available data via the EpiR package in R.¹⁵

^c NPV was reported as 97% in the publication, but was calculated as 98% via the EpiR package in R.¹⁵

^d Patient eligibility was determined using the results of the index test (i.e., only patients who tested positive using the index test at a relative vessel density of 60% or less were included); as such, the values for sensitivity and specificity were not calculated as the sample was selected to exclude any true negatives and false negatives.

Table 27: Study Results, by Outcome — Diagnostic Accuracy for the Detection of ICH

Study Citation	Index Test and Reference Standard	TP	FP	FN	TN	Sensitivity (95% CI)	Specificity (95% CI)	PPV (95% CI)	NPV (95% CI)	AUC
Eldaya et al. (2022) ¹¹ (N = 307)	IT: Rapid ICH + neuroradiologist RS: Either a neuroradiologist (in the case of concordance) or a consensus panel of 3 neuroradiologists (in the case of discordance)	34	1	3	269	92% (78 to 98)	100% (98 to 100)	97% (85 to 100)	99% (97 to 100)	NR

AUC = area under the receiver operating characteristic curve; FN = false negatives; FP = false positives; ICH = intracranial hemorrhage; IT = index test; NPV = negative predictive value; NR = not reported; PPV = positive predictive value; TN = true negatives; TP = true positives; RS = reference standard.

DRAFT

Reasons for Certainty of Evidence Ratings

Table 28: Certainty of Evidence Ratings for CTA With RapidAI Versus CTA Without RapidAI for People With Suspected Acute Stroke

Outcome	Certainty	Reason for Rating
Time to intervention		
Radiology report turnaround	Low <i>(due to risk of bias)</i>	Due to the NRS design and critical risk of bias due to baseline confounding as assessed via ROBINS-I, the certainty of evidence was started at low. We based our judgment of imprecision on the optimal information size, which was exceeded.
Door to intervention	Very low <i>(due to risk of bias and imprecision)</i>	Due to the NRS design and serious risk of bias due to baseline confounding as assessed via ROBINS-I, the certainty of evidence was started at low. Rated down 1 level for serious imprecision due to the small sample size.
CTA to groin puncture	Very low <i>(due to risk of bias and imprecision)</i>	Due to the NRS design and serious risk of bias due to baseline confounding as assessed via ROBINS-I, the certainty of evidence was started at low. Rated down 1 level for serious imprecision due to the small sample size.
Functional status		
Neurological deficit (per NIHSS score)	Very low <i>(due to risk of bias and imprecision)</i>	Due to the NRS design and serious risk of bias due to baseline confounding as assessed via ROBINS-I, the certainty of evidence was started at low. Rated down 1 level for serious imprecision due to the small sample size
Proportion of patients with significant morbidity or mortality (defined as mRS score ≥ 5) at discharge	Very low <i>(due to risk of bias and imprecision)</i>	Due to the NRS design and serious risk of bias due to baseline confounding as assessed via ROBINS-I, the certainty of evidence was started at low. Rated down 2 levels for very serious imprecision. Using the null as the threshold, the 95% CI included the possibility of no difference and benefit.
Disability and dependence in daily activities (per 90-day mRS score)	Very low <i>(due to risk of bias and imprecision)</i>	Due to the NRS design and serious risk of bias due to baseline confounding as assessed via ROBINS-I, the certainty of evidence was started at low. Rated down 1 level for serious imprecision due to the small sample size
Proportion of patients considered to be functionally independent (defined as mRS score ≤ 2) at 90 days	Very low <i>(due to risk of bias and imprecision)</i>	Due to the NRS design and serious risk of bias due to baseline confounding as assessed via ROBINS-I, the certainty of evidence was started at low. Rated down 2 levels for very serious imprecision. Using the null as the threshold, the 95% CI included the possibility of no difference and harm.
Response to therapy		
Proportion of patients with TICI scores of 0, 1, 2A, 2B/C, or 3	Very low <i>(due to risk of bias and imprecision)</i>	Due to the NRS design and serious risk of bias due to baseline confounding as assessed via ROBINS-I, the certainty of evidence was started at low. Rated down 1 level for serious imprecision due to the small sample size.
Patient Harms		
NR	NA	NA

CI = confidence interval; CTA = computed tomography angiography; mRS = modified Rankin Scale; NA = not applicable; NIHSS = National Institutes of Health Stroke Scale; NR = not reported; TICI = Thrombolysis in Cerebral Infarction.

Source: Soun et al. (2023)² and Adhya et al. (2021).²



Table 29: Certainty of Evidence Ratings for the Diagnostic Accuracy of RapidAI with Clinician Interpretation Relative to Clinician Interpretation (or Clinician Consensus) for Suspected Acute Stroke

Index Test	Certainty	Reason for Rating
ICH		
Rapid ICH (version NR) with interpretation by a neuroradiologist	Low <i>(due to risk of bias and imprecision)</i>	Serious risk of bias, as all contributing studies were at high risk as assessed via QUADAS-2. Serious imprecision, as the ranges of the 95% CIs included values that may lead to different conclusions about value of the index test (i.e., values both above and below a sensitivity or specificity of 90%, a threshold suggested by a clinical expert that we consulted for this project)

CI = confidence interval; ICH = intracranial hemorrhage; NR = not reported; QUADAS-2 = Quality Assessment of Diagnostic Accuracy Studies 2.

Source: Eldaya et al. (2022).¹¹

Table 30: Certainty of Evidence Ratings for the Diagnostic Accuracy of RapidAI Alone Relative to Clinician Interpretation (or Clinician Consensus) for Suspected Acute Stroke

Index Test	Certainty	Reason for Rating
M1 MCA and ICA LVO		
Rapid LVO (RapidAI v4.9) alone	Low <i>(due to risk of bias and imprecision)^b</i>	Rated down 1 level for serious risk of bias, as all contributing studies were at high risk as assessed via QUADAS-2. Rated down 1 level for serious imprecision, as the ranges of the 95% CIs included values that may lead to different conclusions about value of the index test (i.e., values both above and below a sensitivity or specificity of 90%, a threshold suggested by a clinical expert that we consulted for this project). The 95% CI for 1 study was neither reported nor calculable, precluding a comprehensive judgment about the precision of the estimates.
Rapid LVO (v1.0) alone	Moderate <i>(due to risk of bias)^d</i>	Rated down 1 level for serious risk of bias, as all contributing studies were at high risk as assessed via QUADAS-2.
Rapid CTA (RapidAI v4.9) alone	Moderate <i>(due to imprecision)^e</i>	Rated down 1 level for serious imprecision, as the ranges of the 95% CIs included values that may lead to different conclusions about value of the index test (i.e., values both above and below a sensitivity or specificity of 90%, a threshold suggested by a clinical expert that we consulted for this project)
Rapid CTA (version NR) alone	Low <i>(due to risk of bias and imprecision)^f</i>	Rated down 1 level for serious risk of bias, as all contributing studies were at high risk as assessed via QUADAS-2. Rated down 1 level for serious imprecision, as the ranges of the 95% CIs included values that may lead to different conclusions about value of the index test (i.e., values both above and below a sensitivity or specificity of 90%, a threshold suggested by a clinical expert that we consulted for this project).
Rapid NCCT Stroke platform (version NR) alone ^g	Low <i>(due to risk of bias and imprecision)^f</i>	Rated down 1 level for serious risk of bias, as all contributing studies were at high risk as assessed via QUADAS-2. Rated down 1 level for serious imprecision, as the ranges of the 95% CIs included values that may lead to different conclusions about value of the index test (i.e., values both above and below a sensitivity or specificity of 90%, a threshold suggested by a clinical expert that we consulted for this project).
M1 and M2 MCA and ICA LVO		
RapidAI alone (version NR)	Low <i>(due to risk of bias and imprecision)^f</i>	Rated down 1 level for serious risk of bias, as all contributing studies were at high risk as assessed via QUADAS-2. Rated down 1 level for serious imprecision, as the ranges of the 95% CIs included values that may lead to different conclusions about value of the index test (i.e., values both above and below a sensitivity or specificity of 90%, a threshold suggested by a clinical expert that we consulted for this project).
Rapid CTA alone (RapidAI v4.9)	Low <i>(due to risk of bias and imprecision)^f</i>	Rated down 1 level for serious risk of bias, as all contributing studies were at high risk as assessed via QUADAS-2. Rated down 1 level for serious imprecision, as the ranges of the 95% CIs included values that may lead to different conclusions about



Index Test	Certainty	Reason for Rating
		value of the index test (i.e., values both above and below a sensitivity or specificity of 90%, a threshold suggested by a clinical expert that we consulted for this project).
M1 MCA LVO		
RapidAI alone (version NR)	Low <i>(due to risk of bias and imprecision)^f</i>	Rated down 1 level for serious risk of bias, as all contributing studies were at high risk as assessed via QUADAS-2. Rated down 1 level for serious imprecision, as the ranges of the 95% CIs included values that may lead to different conclusions about value of the index test (i.e., values both above and below a sensitivity or specificity of 90%, a threshold suggested by a clinical expert that we consulted for this project).
Rapid LVO alone (as part of RapidAI v4.9)	Low <i>(due to risk of bias and imprecision)^f</i>	Rated down 1 level for serious risk of bias, as all contributing studies were at high risk as assessed via QUADAS-2. Rated down 1 level for serious imprecision, as the ranges of the 95% CIs included values that may lead to different conclusions about value of the index test (i.e., values both above and below a sensitivity or specificity of 90%, a threshold suggested by a clinical expert that we consulted for this project).
M2 MCA LVO		
Rapid LVO (RapidAI v4.9) alone	Insufficient information to judge ^h	The certainty of evidence could not comprehensively be judged owing to incomplete reporting in the study. The number of false negatives and true negatives, the specificity, and the 95% CIs for sensitivity were neither reported nor calculable. The study was at high risk of bias as assessed via QUADAS-2.
Rapid CTA (RapidAI v4.9) alone	Low <i>(due to risk of bias and imprecision)^f</i>	Rated down 1 level for serious risk of bias, as all contributing studies were at high risk as assessed via QUADAS-2. Rated down 1 level for serious imprecision, as the ranges of the 95% CIs included values that may lead to different conclusions about value of the index test (i.e., values both above and below a sensitivity or specificity of 90%, a threshold suggested by a clinical expert that we consulted for this project).
ICA LVO		
Rapid LVO (RapidAI v4.9) alone	Low <i>(due to risk of bias and imprecision)^f</i>	Rated down 1 level for serious risk of bias, as all contributing studies were at high risk as assessed via QUADAS-2. Rated down 1 level for serious imprecision, as the ranges of the 95% CIs included values that may lead to different conclusions about value of the index test (i.e., values both above and below a sensitivity or specificity of 90%, a threshold suggested by a clinical expert that we consulted for this project).
LVO of the ICA, M1 or M2 MCA, basilar artery, or intracranial vertebral artery		
Rapid LVO alone (RapidAI v5.1)	Low <i>(due to risk of bias and imprecision)^f</i>	Rated down 1 level for serious risk of bias, as all contributing studies were at high risk as assessed via QUADAS-2. Rated down 1 level for serious imprecision, as the ranges of the 95% CIs included values that may lead to different conclusions about value of the index test (i.e., values both above and below a sensitivity or specificity of 90%, a threshold suggested by a clinical expert that we consulted for this project).
Undefined LVO^a		
Rapid LVO (v5.2.2) alone	Low <i>(due to risk of bias and imprecision)^f</i>	Rated down 1 level for serious risk of bias, as all contributing studies were at high risk as assessed via QUADAS-2. Rated down 1 level for serious imprecision, as the ranges of the 95% CIs included values that may lead to different conclusions about value of the index test (i.e., values both above and below a sensitivity or specificity of 90%, a threshold suggested by a clinical expert that we consulted for this project).
Rapid CTA (version NR) alone at < 45% relative vessel density threshold	Very low <i>(due to risk of bias and imprecision)^j</i>	Rated down 2 levels for very serious risk of bias, as all contributing studies were at high risk with concerns related to patient selection as assessed via QUADAS-2. Patient eligibility was determined using the results of the index test (i.e., only patients who tested positive using the index test at a relative vessel density of 60% or less were included); as such, the values calculated for sensitivity and specificity are drawn from a sample of patients that is not representative of clinical practice (as the sample excludes anyone with a relative vessel density of greater than 60%). Rated down 1 level for serious imprecision, as the ranges of the 95% CIs included values that may lead to different conclusions about value of the index test (i.e.,



Index Test	Certainty	Reason for Rating
		values both above and below a sensitivity or specificity of 90%, a threshold suggested by a clinical expert that we consulted for this project).

CI = confidence interval; CTA = computed tomography angiography; ICA = internal carotid artery; LVO = large vessel occlusion; MCA = middle cerebral artery; NCCT = non-contrast computed tomography; NR = not reported; QUADAS-2 = Quality Assessment of Diagnostic Accuracy Studies 2.

^a Unclear which types of LVO were considered eligible. In Delora et al. (2024), the study population included patients with occlusions of the ICA, M1 MCA segment, and M2 MCA segment. The study population from Adhya et al. (2021) included patients with occlusions of the ICA, carotid terminus, M1 MCA segment, and M2 MCA segment.

Source: Delora et al. (2024),³ Slater et al. (2024),⁴ Chan et al. (2023),⁵ Soun et al. (2023),¹ Yedavalli et al. (2023),⁶ Mallon et al. (2022),⁷ Schlossman et al. (2022),⁸ Adhya et al. (2021),² Dehkharghani et al. (2021),⁹ and Amukotuwa et al. (2019).¹⁰

DRAFT

Patient Engagement

Table 31: Summary of Patient Engagement Using the Guidance for Reporting Involvement of Patients and the Public (version 2) Short Form Reporting Checklist¹⁶

Section and topic	Item	Report section
Aim	One patient contributor participated in a 1-hour interview during the drafting phase of the report to highlight her experiences, perspectives, and priorities for the use of AI in stroke detection.	Methods
Methods	After giving informed consent, 1 patient contributor discussed her experience of a stroke and her perspectives on the use of AI in stroke detection.	Methods
Results of engagement	<p>Perspectives Shared</p> <p>The patient contributor shared her personal experience of having a hemorrhagic stroke, the emergency treatment she received, and her recovery. She did not know whether AI had been used in her diagnosis.</p> <p>RapidAI</p> <p>RapidAI was described to the patient contributor, and she shared her thoughts on its use in stroke detection, relating to perceived potential outcomes and ethical considerations as described below.</p> <p>Outcomes to Measure</p> <p><i>Speed</i></p> <p>Two of the potential benefits that the patient contributor hoped for was speed and accuracy. She was hopeful that if the use of AI meant a speedier and more accurate diagnosis, perhaps clinicians could initiate the most appropriate treatment sooner. She hoped that this would reduce the damage being caused by the stroke and improve outcomes.</p> <p><i>Accuracy</i></p> <p>When asked to expand on her comment about accuracy being crucial to the success of using AI, the patient contributor posited that, while ensuring the accuracy of the AI technology was a concern, she was curious about whether AI could accurately identify issues earlier than a clinician, or perhaps prevent human error.</p> <p><i>Other Outcomes</i></p> <p>When asked specifically about outcomes of interest, speed and accuracy were the patient contributor's priorities. However, she also identified minimizing the damage caused by strokes and mortality rates as other factors to consider.</p> <p>Ethical Considerations</p> <p><i>Equitable Access</i></p> <p>The patient contributor expressed concern about the accessibility of RapidAI technologies outside of major stroke centres and wondered whether all major hospitals could benefit from this technology to assist in triaging (and potentially transferring) patients more quickly. She also had concerns about services in rural and remote community hospitals.</p> <p><i>Privacy</i></p>	Summary of Evidence



Section and topic	Item	Report section
	<p>The patient contributor suggested that, in a crisis, she felt that most people wouldn't be thinking of ethical considerations like privacy and data sharing – they would be focused on diagnosis, treatment, and survival.</p> <p>The patient contributor reflected that some people may be more reluctant to have their personal information shared with the manufacturer, while others may be used to sharing their personal information with cell phone or computer software manufacturers. She suggested that there may be a divide, with some individuals being more protective of their personal information and others more familiar with novel technologies and sharing their data.</p> <p>Regardless of the level of patient comfort with sharing data, the patient contributor shared concerns about privacy, safety of information, accuracy, and reliability of storage.</p> <p><i>Informing the Patient</i></p> <p>The patient contributor expressed curiosity about whether patients will be informed that their clinicians used AI in their diagnosis. She herself did not know whether the technology was in use at the time of her stroke.</p>	
Discussion and conclusions	<p>Success of engagement in this review is related to several factors. Firstly, there was outreach through several organizations. Secondly, the patient contributor was briefed on the objectives of the project in an introductory call and supported by a Patient Engagement Officer. Thirdly, 3 of the project team members attended the interview to hear from the individual directly and to engage her in conversation. Fourthly, a gift card was offered as a gesture of appreciation for her contribution. Finally, the patient contributor was offered the opportunity to be thanked by name in the acknowledgements section of the report or to remain anonymous. She preferred to remain anonymous.</p> <p>However, there were limitations. Though we had intended to engage with 3 individuals, 2 patients and a clinician, we had limited response to our outreach, and the sole clinician who responded to our initial request ultimately declined to participate due to time constraints.</p>	Summary of Evidence
Critical Reflections	<p>The patient contributor was highly engaged in the discussion, sharing her experience, thoughts, and priorities. Questions were sent ahead of time so that she could prepare. A summary of the discussion was drafted and sent to the patient contributor. She was able to share feedback and approve the summary as an accurate reflection of the conversation.</p> <p>One limitation of our approach is that people need access to reliable technology, phone, and internet access to contribute to our work, which may exclude some voices.</p>	NA

AI = artificial intelligence; NA = not applicable.

References

1. Soun JE, Zolyan A, McLouth J, et al. Impact of an automated large vessel occlusion detection tool on clinical workflow and patient outcomes. *Front Neurol.* 2023;14:1179250.
2. Adhya J, Li C, Eisenmenger L, et al. Positive predictive value and stroke workflow outcomes using automated vessel density (RAPID-CTA) in stroke patients: One year experience. *Neuroradiol J.* 2021;34(5):476-481.
3. Delora A, Hadjialiakbari C, Percenti E, et al. Viz LVO versus Rapid LVO in detection of large vessel occlusion on CT angiography for acute stroke. *J Neurointerv Surg.* 2024;16(6):599-602.
4. Slater LA, Ravintharan N, Goergen S, et al. *RapidAI* Compared With Human Readers of Acute Stroke Imaging for Detection of Intracranial Vessel Occlusion. *Stroke: Vascular and Interventional Neurology.* 2024;4(2):e001145.
5. Chan N, Sibtain N, Booth T, et al. Machine-learning algorithm in acute stroke: real-world experience. *Clin Radiol.* 2023;78(2):e45-e51.
6. Yedavalli V, Heit JJ, Dehkharghani S, et al. Performance of RAPID noncontrast CT stroke platform in large vessel occlusion and intracranial hemorrhage detection. *Front Neurol.* 2023;14:1324088.
7. Mallon DH, Taylor EJR, Vittay OI, Sheeka A, Doig D, Lobotesis K. Comparison of automated ASPECTS, large vessel occlusion detection and CTP analysis provided by Brainomix and RapidAI in patients with suspected ischaemic stroke. *J Stroke Cerebrovasc Dis.* 2022;31(10):106702.
8. Schlossman J, Ro D, Salehi S, et al. Head-to-head comparison of commercial artificial intelligence solutions for detection of large vessel occlusion at a comprehensive stroke center. *Front Neurol.* 2022;13:1026609.
9. Dehkharghani S, Lansberg M, Venkatsubramanian C, et al. High-Performance Automated Anterior Circulation CT Angiographic Clot Detection in Acute Stroke: A Multireader Comparison. *Radiology.* 2021;298(3):665-670.
10. Amukotuwa SA, Straka M, Smith H, et al. Automated Detection of Intracranial Large Vessel Occlusions on Computed Tomography Angiography: A Single Center Experience. *Stroke.* 2019;50(10):2790-2798.
11. Eldaya RW, Kansagra AP, Zei M, et al. Performance of Automated RAPID Intracranial Hemorrhage Detection in Real-World Practice: A Single-Institution Experience. *Journal of Computer Assisted Tomography.* 2022;46(5):770-774.
12. Brott T, Adams HP, Olinger CP, et al. Measurements of acute cerebral infarction: a clinical examination scale. *Stroke.* 1989;20(7):864-870.
13. Banks JL, Marotta CA. Outcomes Validity and Reliability of the Modified Rankin Scale: Implications for Stroke Clinical Trials. *Stroke.* 2007;38(3):1091-1096.
14. Goyal M, Fargen KM, Turk AS, et al. 2C or not 2C: defining an improved revascularization grading scale and the need for standardization of angiography outcomes in stroke trials. *J Neurointerv Surg.* 2014;6(2):83-86.
15. Stevenson M, Sergeant E. epiR: Tools for the Analysis of Epidemiological Data. R package version 2.0.74. 2024; <https://CRAN.R-project.org/package=epiR>. Accessed 2024 Jun 5.
16. Staniszewska S, Brett J, Simera I, et al. GRIPP2 reporting checklists: tools to improve reporting of patient and public involvement in research. *BMJ.* 2017;358:j3453.



ISSN: TBD

Disclaimer: The information in this document is intended to help Canadian health care decision-makers, health care professionals, health systems leaders, and policy-makers make well-informed decisions and thereby improve the quality of health care services. While patients and others may access this document, the document is made available for informational purposes only and no representations or warranties are made with respect to its fitness for any particular purpose. The information in this document should not be used as a substitute for professional medical advice or as a substitute for the application of clinical judgment in respect of the care of a particular patient or other professional judgment in any decision-making process. The Canadian Agency for Drugs and Technologies in Health (CADTH) does not endorse any information, drugs, therapies, treatments, products, processes, or services.

While care has been taken to ensure that the information prepared by CADTH in this document is accurate, complete, and up to date as at the applicable date the material was first published by CADTH, CADTH does not make any guarantees to that effect. CADTH does not guarantee and is not responsible for the quality, currency, propriety, accuracy, or reasonableness of any statements, information, or conclusions contained in any third-party materials used in preparing this document. The views and opinions of third parties published in this document do not necessarily state or reflect those of CADTH.

CADTH is not responsible for any errors, omissions, injury, loss, or damage arising from or relating to the use (or misuse) of any information, statements, or conclusions contained in or implied by the contents of this document or any of the source materials.

This document may contain links to third-party websites. CADTH does not have control over the content of such sites. Use of third-party sites is governed by the third-party website owners' own terms and conditions set out for such sites. CADTH does not make any guarantee with respect to any information contained on such third-party sites and CADTH is not responsible for any injury, loss, or damage suffered as a result of using such third-party sites. CADTH has no responsibility for the collection, use, and disclosure of personal information by third-party sites.

Subject to the aforementioned limitations, the views expressed herein are those of CADTH and do not necessarily represent the views of Canada's federal, provincial, or territorial governments or any third-party supplier of information.

This document is prepared and intended for use in the context of the Canadian health care system. The use of this document outside of Canada is done so at the user's own risk.

This disclaimer and any questions or matters of any nature arising from or relating to the content or use (or misuse) of this document will be governed by and interpreted in accordance with the laws of the Province of Ontario and the laws of Canada applicable therein, and all proceedings shall be subject to the exclusive jurisdiction of the courts of the Province of Ontario, Canada.

The copyright and other intellectual property rights in this document are owned by CADTH and its licensors. These rights are protected by the Canadian *Copyright Act* and other national and international laws and agreements. Users are permitted to make copies of this document for non-commercial purposes only, provided it is not modified when reproduced and appropriate credit is given to CADTH and its licensors.

About CADTH: CADTH is an independent, not-for-profit organization responsible for providing Canada's health care decision-makers with objective evidence to help make informed decisions about the optimal use of drugs, medical devices, diagnostics, and procedures in our health care system.

Funding: CADTH receives funding from Canada's federal, provincial, and territorial governments, with the exception of Quebec.

Questions or requests for information about this report can be directed to Requests@CADTH.ca